



# Digital Sight series

Digital Cameras for Microscopes



# Nikon Digital Sight Series

Newly added a model that boasts ultra-high-definition, a wide field of view, and high sensitivity

With various models, including the ultra-high-definition monochrome camera Digital Sight 50M and Digital Sight 10, which can switch between color and monochrome, you can choose the microscope camera for your particular purpose.

Attention: All the examples in this page are images for research. We do not guarantee clinical use.

Four camera options covering two computing platforms

Microscope Camera <b>Digital Sight 1000</b>	Microscope Camera <b>DS-Fi3</b>	Microscope Camera <b>Digital Sight 10</b>	Monochrome Microscope Camera <b>Digital Sight 50M</b> <span style="color:red">NEW</span>
			
→ P.3	→ P.4	→ P.8	→ P.12
2.0 megapixel Color Full HD	5.9 megapixel Color High-resolution	23.9 megapixel Color/Mono-chrome High-resolution	60.0 megapixel Mono-chrome Cooled
Frame rate 30 fps (1920×1080)	Frame rate 15 fps (2880×2048), 30 fps (1440×1024)	Frame rate 9 fps (6000×3984), 66 fps (1920×1080)	Frame rate 6 fps (9552×6336), 225.9 fps (640×480)
Max recordable pixels 1920×1080	Max recordable pixels 2880×2048	Max recordable pixels 6000×3984	Max recordable pixels 9552×6336
C-Mount	C-Mount	F-Mount	F-Mount

**Using a tablet PC**

Imaging software  
**NIS-Elements**  
Advanced Solutions for your Imaging World



→ P.18

**Using a desktop PC**

Imaging software  
**NIS-Elements**  
Advanced Solutions for your Imaging World




\*Digital Sight 1000 is only compatible with NIS-Elements F.

→ P.16

## Microscope Camera

# Digital Sight 1000

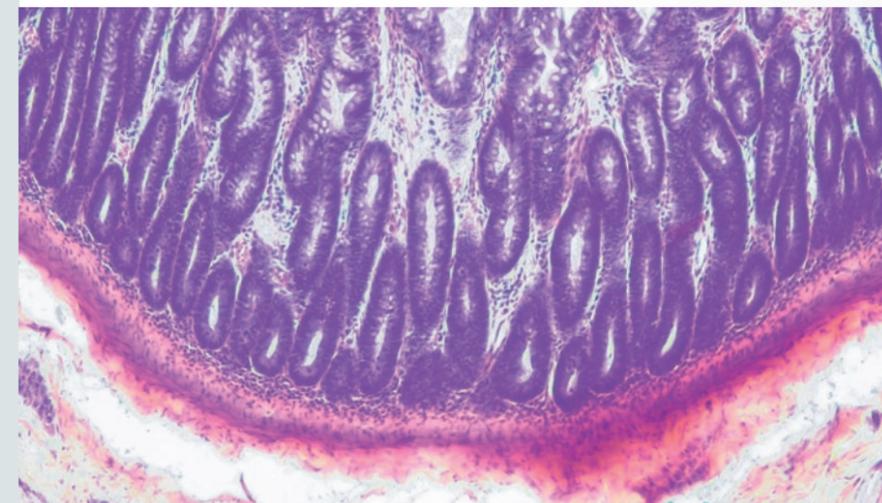


## Full HD images

Equipped with a 2 megapixel CMOS image sensor, the Digital Sight 1000 can display, capture and save full HD, 1920×1080 pixel images at 30 frames / second.

## Stand-alone mode

By connecting a Full HD display and a mouse, the Digital Sight 1000 can be used without a PC, conserving bench space. Captured images and videos can be saved directly to an SD card which is inserted into the camera. Users can easily display scale bars, measure areas and calculate distances between two points.

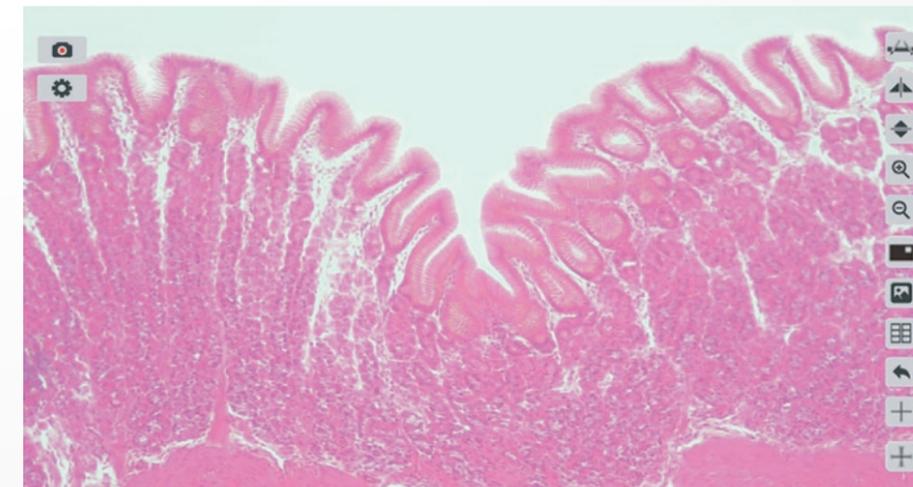


## Microscope Camera DS-Fi3



### High-resolution images



A CMOS high density 5.9 megapixel sensor produces high resolution images. USB3.0 data transfer allows fast focusing at high resolution, and easy capture images in all types of observation methods such as brightfield, differential interference contrast, and phase contrast.

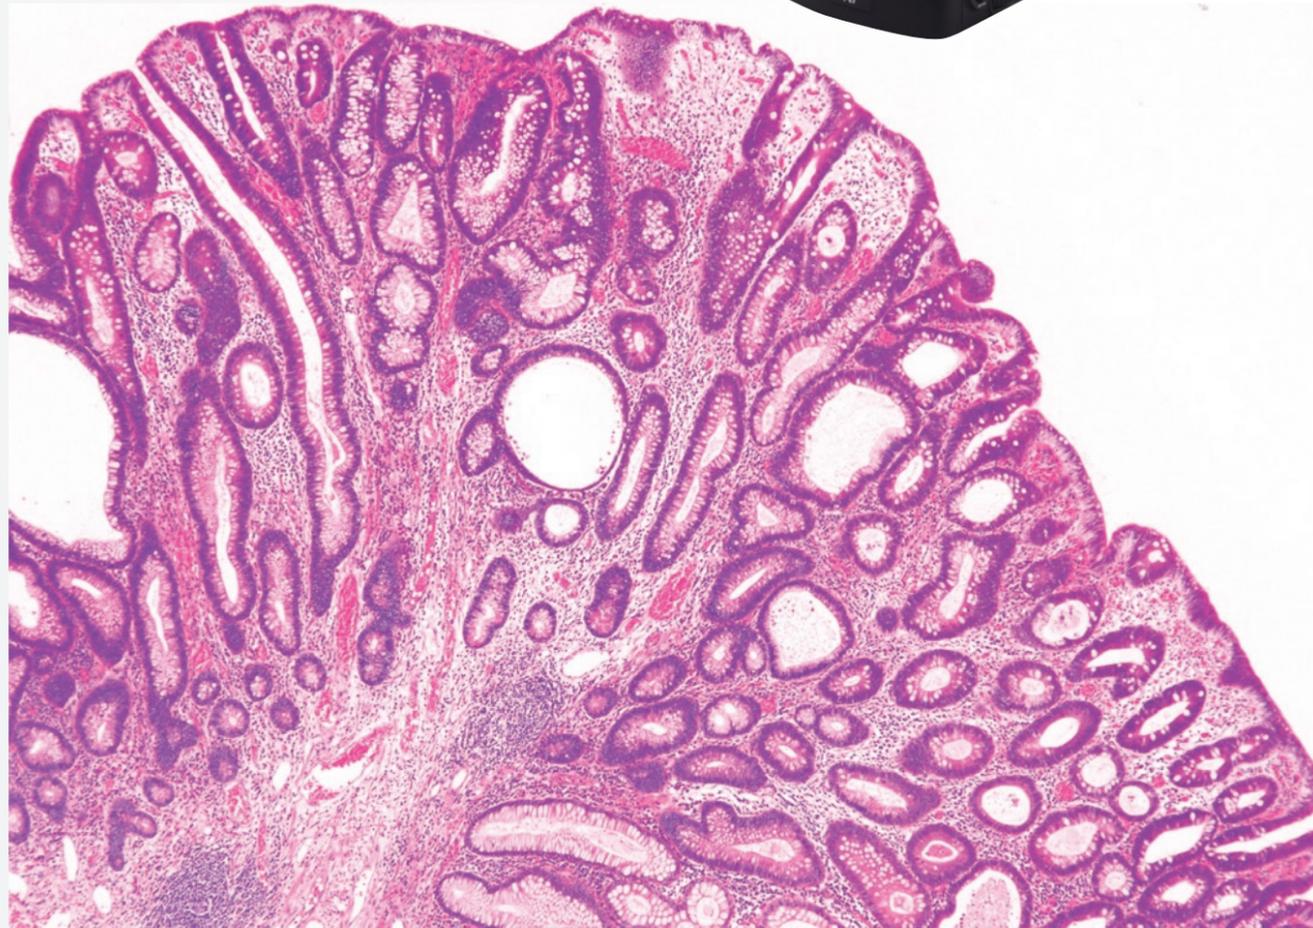

Tubular adenoma, HE staining (Objective: CFI Plan Apochromat Lambda 4X)  
Photos courtesy of: Dr. Yasunori Ohta, Department of Pathology, IMSUT Hospital, Institute of Medical Science, The University of Tokyo

### High sensitivity, low noise


Quantum efficiency and read noise have been greatly improved, providing better capability for acquisition of fluorescent images with better signal-to-noise ratios than before.

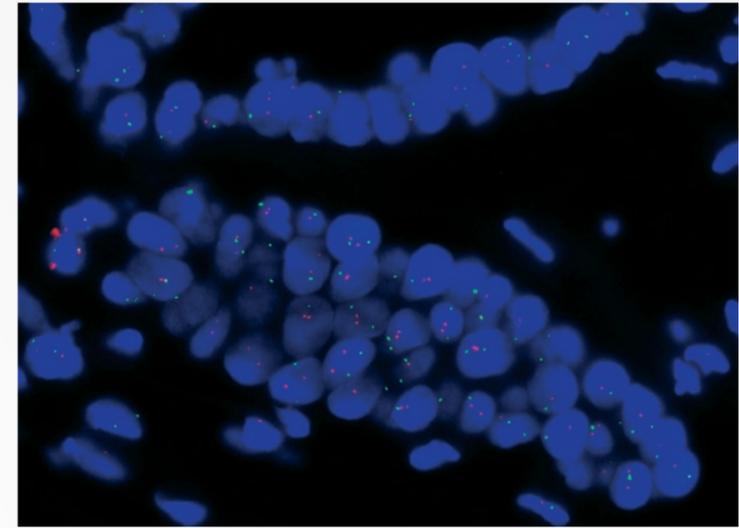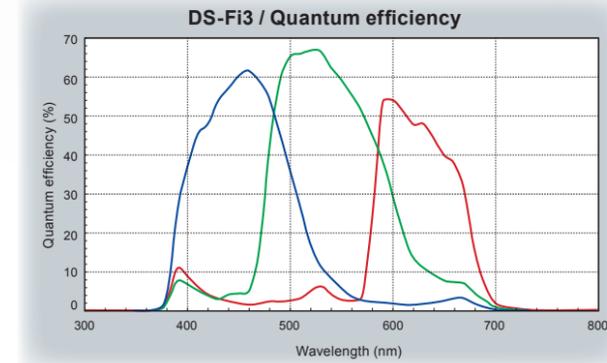


Breast cancer, FISH method (Objective: CFI Plan Apochromat Lambda 100X Oil)  
Photos courtesy of: Hironao Kusakari, Diagnostic Pathology, St. Marianna University Hospital

### Superior color reproduction

Nikon is well-known for outstanding and lifelike color reproduction, and developing superior algorithms for creating results that look like the actual samples. These algorithms are used in all of the color cameras in the digital sight lineup.

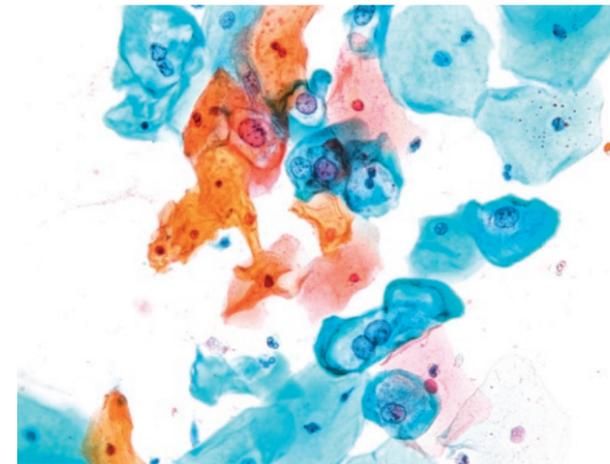

Uterine cervix Pap. Staining  
(Objective: CFI Plan Apochromat Lambda 40XC)  
Photos courtesy of: Kazuhiro Mita, Department of Pathology, Yokohama City University Hospital

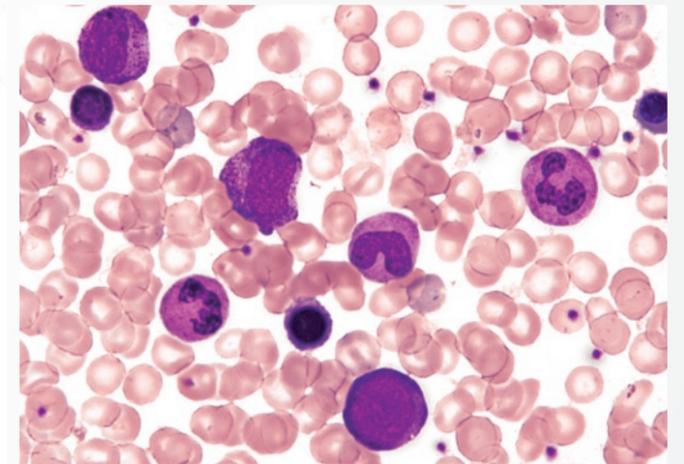

Bone marrow  
(Objective: CFI Plan Achromat NCG 40X)  
Photos courtesy of: Clinical Laboratory Department, Yokohama City University Hospital

### High-speed live display

Fast USB3.0 data transfer means fast, smooth live updating of images for finding samples or focusing, even at full resolution.


### Camera Control

The DS-Fi3 interfaces with PC via a USB3.0 interface directly to the camera head, and uses NIS-Elements series software for image acquisition.

# High-definition cameras Digital Sight 10 & 50M Equipped with Nikon FX format CMOS image sensors

In addition to offering the high definition of 6K, the Digital Sight 10 makes it possible to switch between color and monochrome photography. This is a high-performance model that also offers a high frame rate that can quickly focus for high-definition images.

Providing strong cost performance, the Digital Sight 50M is a cooled, monochrome model that combines 9K image quality, FOV25 wide field of view, and a maximum frame rate of 225.9 fps.

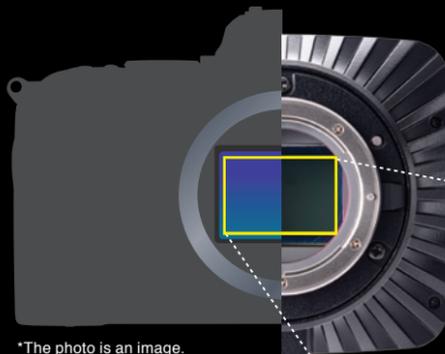

\*The photo is an image.  
It is different from the actual sensor


## Large Format CMOS image sensors

Nikon manufactures CMOS image sensors and imaging technologies for professional DSLR cameras\*, and has optimized our sensors for microscopy.

\*Digital Sight 10 only

## Objective lenses that achieve even higher image quality

Use with the newly developed Plan Apochromat Lambda D series of objective lenses enables the acquisition of even higher quality images.

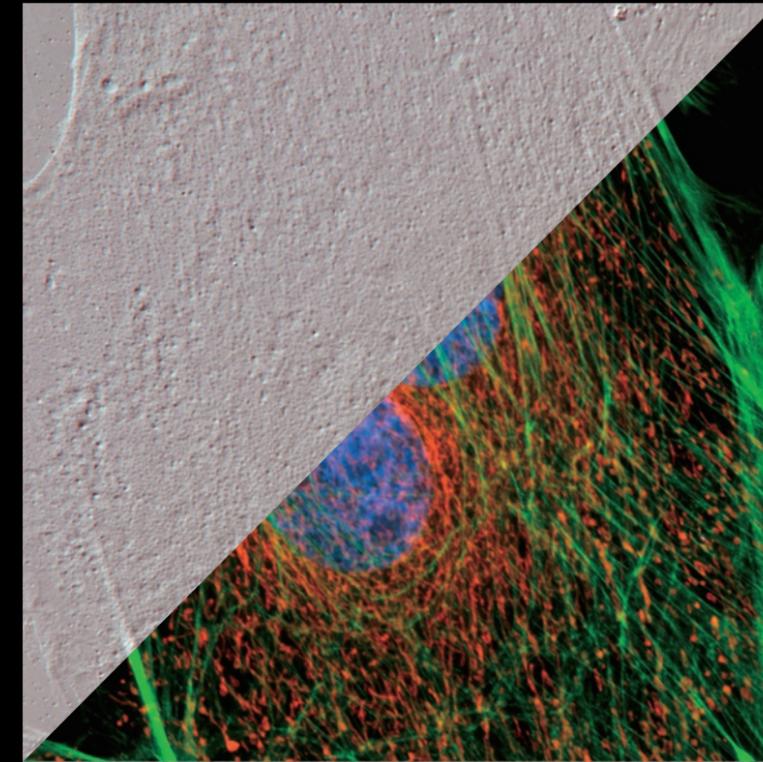


BPAA Fluorescent Stain Specimen Nikon Standard Sample DIC (left) and fluorescence (right)  
Nucleus (DAPI), Actine (FITC), Mitochondria (MitoTracker RedFM)  
Objective: CFI Plan Apochromat Lambda D 100XOil

## Digital Sight 10

Freely switch between color and monochrome at 23.9 megapixels

## Digital Sight 50M

Seamlessly search, capture images of, and analyze samples at high speed

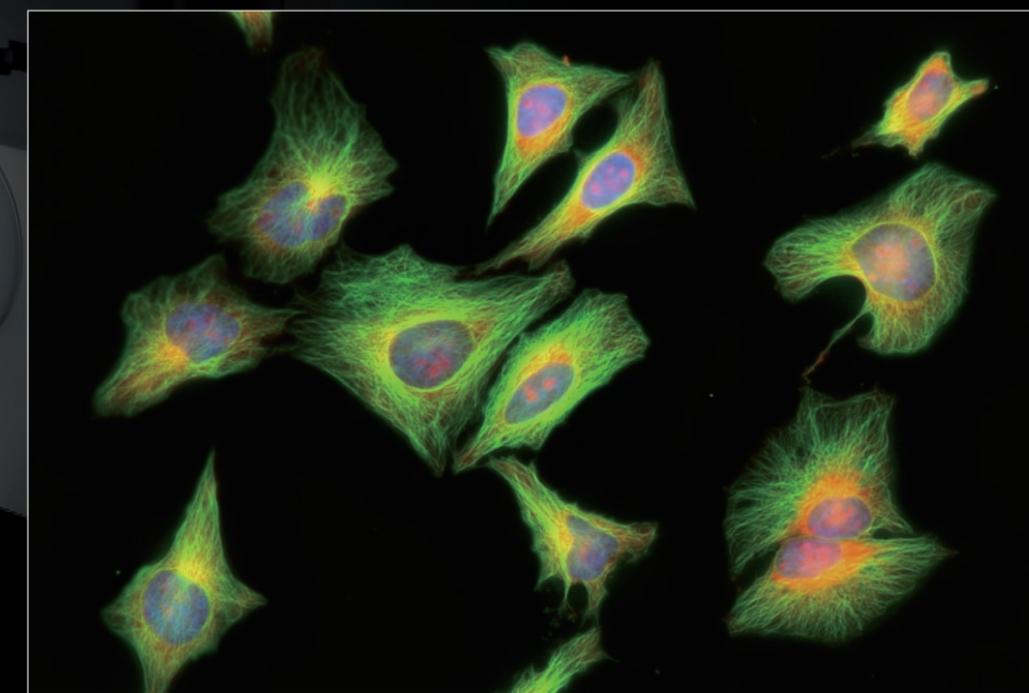

HeLa cells Nucleus (DAPI), Tubulin (FITC), Cell cytoplasm (CellMask™ Red)  
Objective: CFI Plan Apochromat Lambda D 60XOil

Covers a wide field of view with 6K ultra-high Definition. Achieves efficient, one-shot image capture.

Microscope Camera

## Digital Sight 10



23.9 megapixel

Color/Mono-chrome



High-resolution

### Observation with a wide field of view

A full-frame CMOS image sensor for instantaneous one-shot image capture of wide areas

A 25 mm field of view (FOV), possible in combination with inverted microscopes, and upright microscopes, enabling the capture of images over a wider area in one shot. Tiled images can be created efficiently, cutting the time required for screening.

\*Upright microscopes are supported only by the Ni series (brightfield).

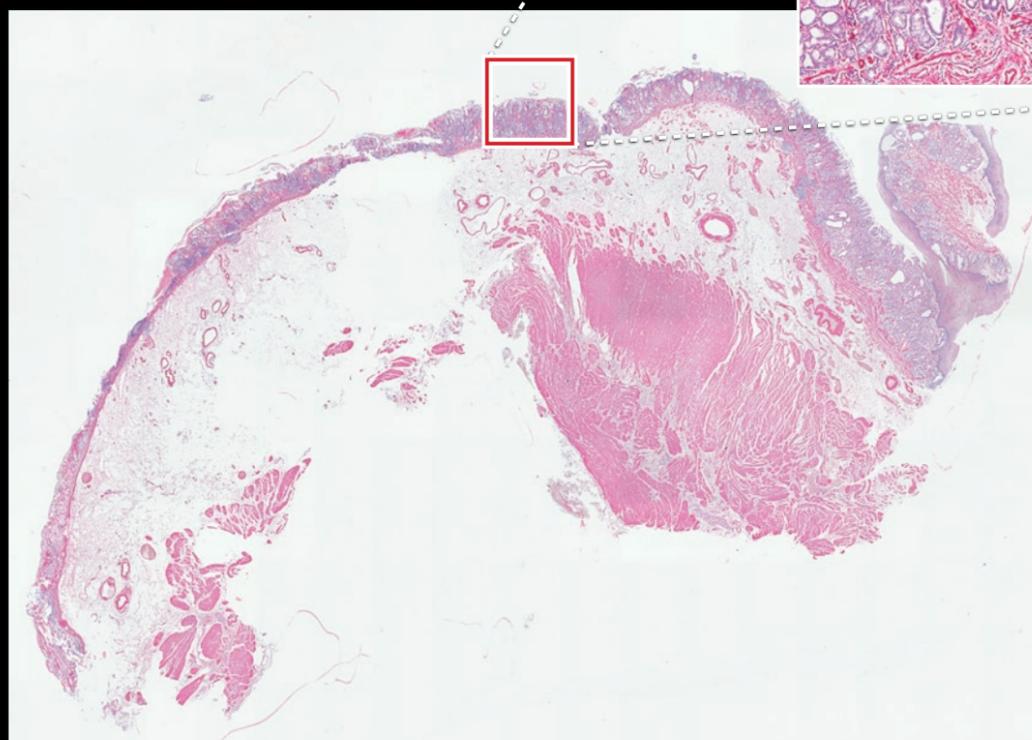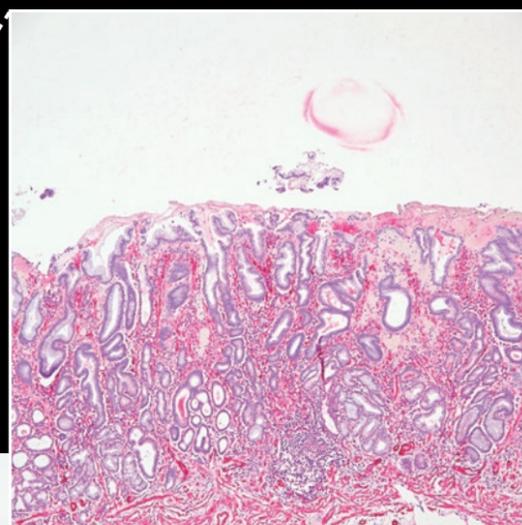


Stomach, SMA staining,  
17x12 Tiled images  
(Objective: CFI Plan  
Apochromat 40XC)  
Photo courtesy of:  
Nichirei Biosciences Inc.

### High-definition observation

Easily capture fine details with 6K pixel resolution and high image quality

Microscopic images can be captured at up to 6000 x 3984 pixels (23.9 megapixels), ideal for image analysis and observation of fine structures.

#### Digital Sight 10

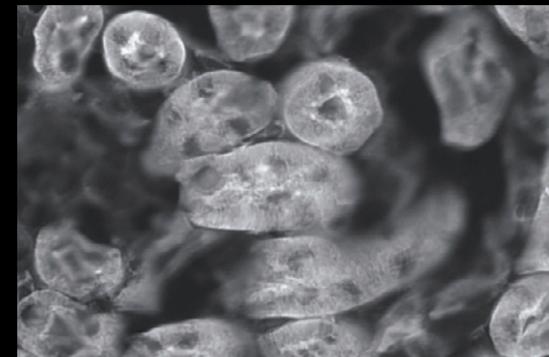

#### Conventional model (DS-Ri2)



Kidney tissue  
(WGA: 488)  
(Objective: CFI Plan  
Apochromat VC 20X)

### Fast live display


A frame rate that captures moving samples at the perfect instant

Digital Sight 10 is capable of live display of 6000 x 3984 pixel (23.9-megapixel) images at 9 frames/second or 1920 x 1080 pixel (2.1-megapixel) images at 66 frames/second. Fine focusing is easy and stress-free. By using the ROI mode, it is possible to shoot only any place at a higher speed.

### High sensitivity and low noise

Ideal for fluorescence observation requiring a wide field of view and high definition

Digital Sight 10 achieves high sensitivity equivalent to ISO 200 in color mode and ISO 800 in monochrome mode. Clear fluorescence observation with a high signal-to-noise ratio is possible in both monochrome and color image acquisition.

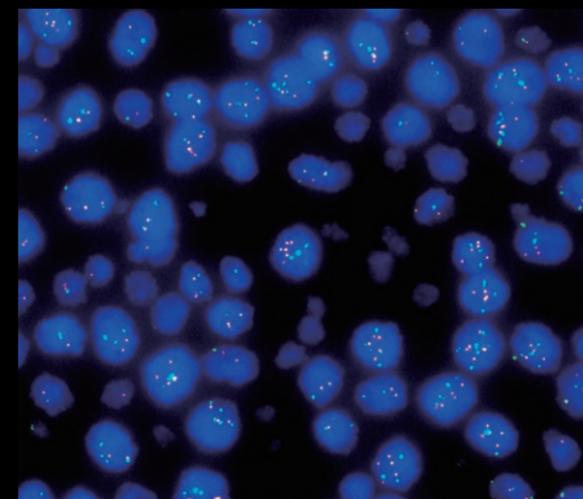

Breast cancer, FISH method (Objective: CFI Plan Apochromat Lambda D 100XOil)  
Photo courtesy of: St. Marianna University Hospital



High-definition capture in both color and monochrome. Ready for use in a wider range of observation scenarios.

**Color shooting and Monochrome shooting are possible with one unit**

During manual operation

**Color mode**



When inserting the color filter  
Can shoot 400 to 680 nm in color

**Monochrome mode**



When detaching the color filter  
Capable of shooting 400 to 850 nm in Monochrome  
\*Replace with monochrome IR filter

**Electric switching function**

During electronic operation (using the 1x electronic adapter)

Easy color mode switching, either manually or electronically

Digital Sight 10 makes it possible to easily switch the color mode either electronically or manually by using specialized imaging software for electronic switching or attaching/detaching filters to the slot at the bottom of the microscope camera for manual switching.




\*A 1x electronic adapter and a separate PC equipped with specialized imaging software, NIS-Elements, are required for electronic operation.

**Achieves consistent shooting with a single sensor**

A convenient all-in-one camera for multiple observation applications

A single sensor captures both color and monochrome images, for consistent appearance even when switching color mode. Easy image acquisition is possible without the hassle of using different cameras.

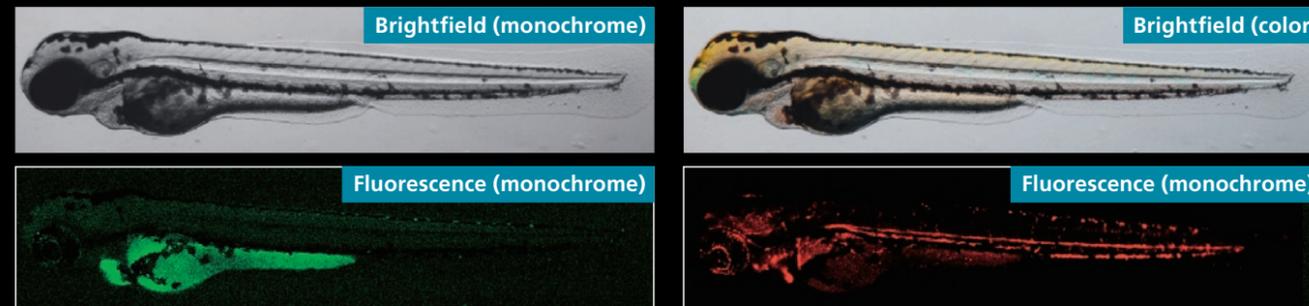

Zebrafish (Objective: SHR Plan Apo 1X)

**A monochrome mode that acquires even near infrared images**

Fluorescence observation with little damage to biological samples

Digital Sight 10's monochrome mode supports near-infrared (700 nm-) fluorescence image capture, normally difficult to achieve with conventional color cameras. As fluorescence sensitivity extends to the NIR region, this camera is suited to fluorescence image capture of thick samples and samples with weak phototoxicity.


**For discriminating fine structures**



Kidney cancer, Vimentin staining (Objective: CFI Plan Apochromat Lambda D 20X)  
Photo courtesy of: Nichirei Biosciences Inc.

Blurring and color bleeding are low even to the periphery, for images that are clear even when enlarged. ECLIPSE Ni supports everyday observation and inspection of samples with high resolution and high color fidelity.

Upright microscope system **ECLIPSE Ni**  
Objective lens for biological microscopes Lambda D

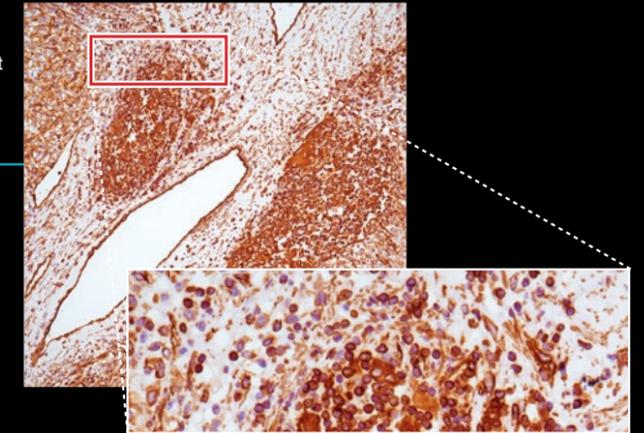


**For 3D imaging**



Mouse neuron (Objective: CFI Plan Apochromat Lambda D 40XC)  
From captured images of 18 μm thickness every 0.2 μm. Image processed with Clarify.ai

ECLIPSE Ti2 takes advantage of a wide field of view (field number 25) to achieve high throughput even when capturing 3D or other large-size data. Combined with image processing, it enables the capture of clear images with a higher signal-to-noise ratio, even deep into subjects.

Inverted microscope system **ECLIPSE Ti2**  
Objective lens for biological microscopes Lambda D

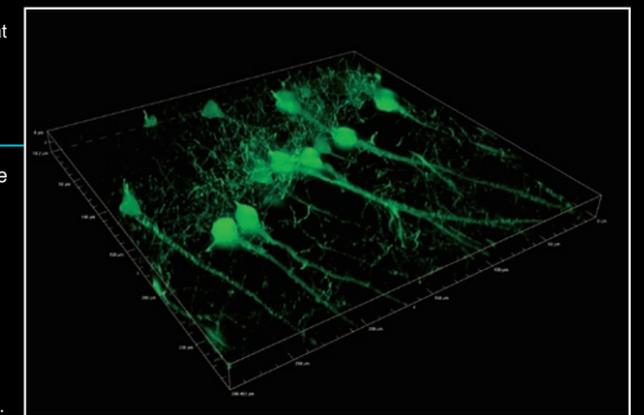

**For model organisms**



Stereoscopic microscope system **SMZ25/18**

Zebrafish larva (brightfield/myocardium GFP) (Objective: SHR Plan Apo 2X)  
Photo courtesy of: Dr. Hiroyuki Nakajima, National Cerebral and Cardiovascular Center

SMZ25/18 offers high definition at high frame rates. Capture perfect, bright images without missing high-speed biological reactions. Low noise makes this system ideal for time lapse imaging.




# Quickly and efficiently search wide fields of view and capture and analyze high-definition images

## Monochrome Microscope Camera Digital Sight 50M



NEW

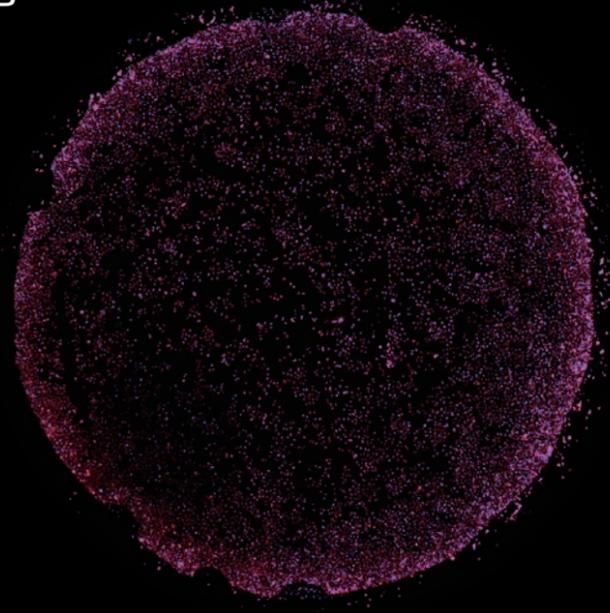

HeLa cells Nucleus(DAPI), Cell cytoplasm(CellMask™DeepRed)  
One-shot shooting of 1 well in a 96-well plate: Ti2-E, CFI Plan Apochromat Lambda D 2X


- 60.0 megapixel
- Mono-chrome
- Cooled

The monochrome digital camera Digital Sight 50M for microscopes is optimized to increase workflow efficiency. In addition to its large number of pixels, number of fields of view, and speed, it comes with dedicated software that makes it effective for screening large volumes of samples. It is perfect for not only academic research but also drug discovery research.

## Dramatically improves the workflow for capturing images of and analyzing large volumes of samples


### Wide field of view and high resolution for single-shot images of individual wells

With an actual field of view of 7 mm when using a 2X objective lens, it is possible to capture single-shot images of wide areas. You can also quickly check both the overall image of large volumes of samples, such as in well plates, and regions of interest of a sample, which increases reproducibility of experiments.

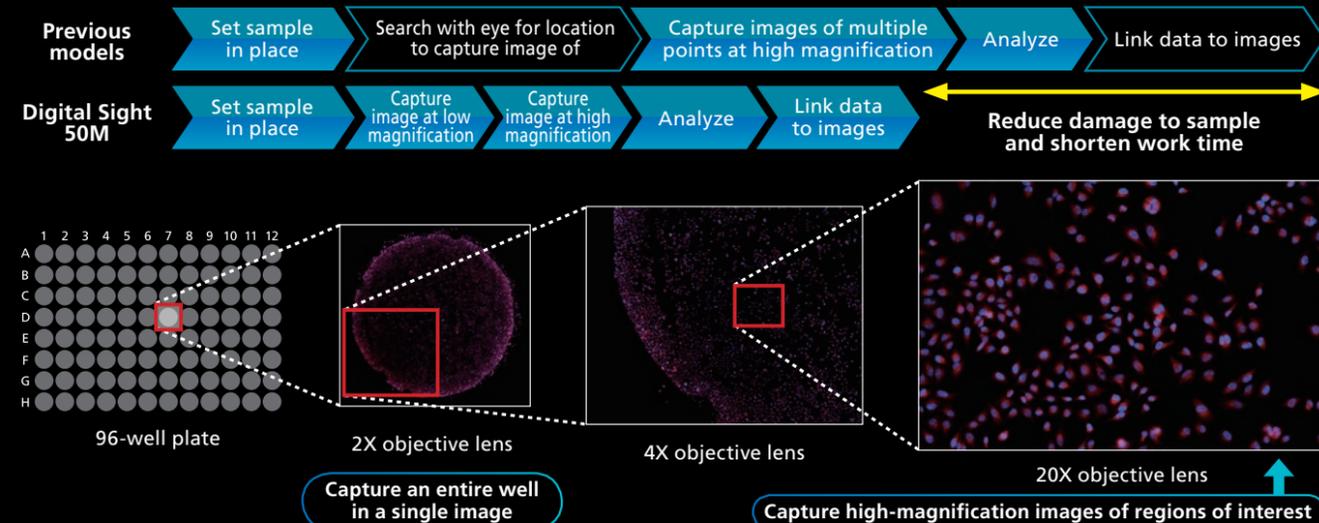


## The ultra-high resolution of 9K increases the reliability of quantitative analysis

The improved Digital Sight 50M boasts 3.8 times the number of pixels and 2.5 times the resolution of previous models. Even when using a low-magnification, high-NA objective lens, it fully demonstrates optical capabilities. It is also possible to obtain highly reliable data of small regions when analyzing images.

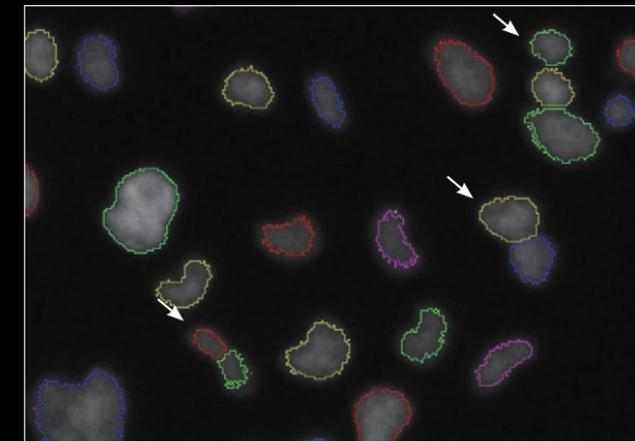


Digital Sight 50M

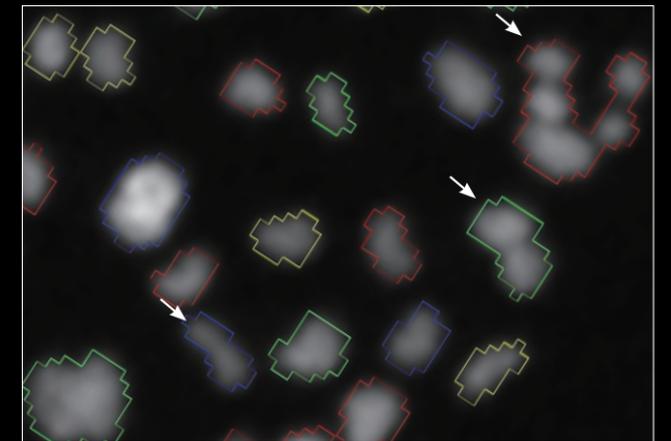


Conventional

## Includes software suited to large-volume screening

The Digital Sight 50M comes with NIS-A Bundle JOBS W/RDB optional software so it offers support through post-capture analysis. It is possible to set up a flow from well selection, automatic detection of image ROI, and displaying of analysis results.

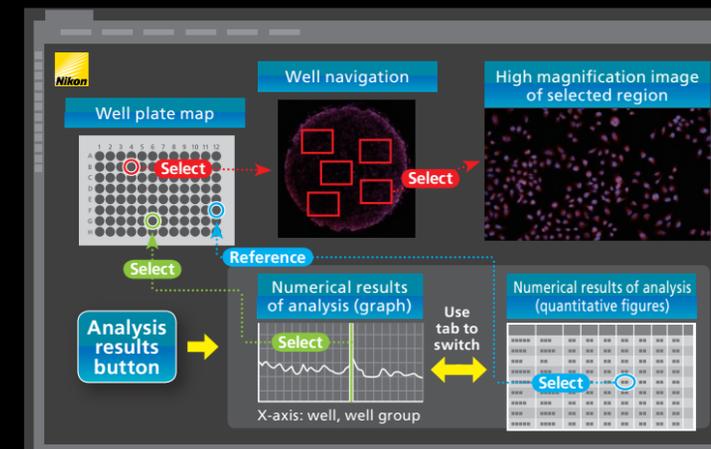


- Plate view
- Heat map
- Sample label
- Binarized image
- Graphs (histogram, scatter plot, bar graph, etc.)

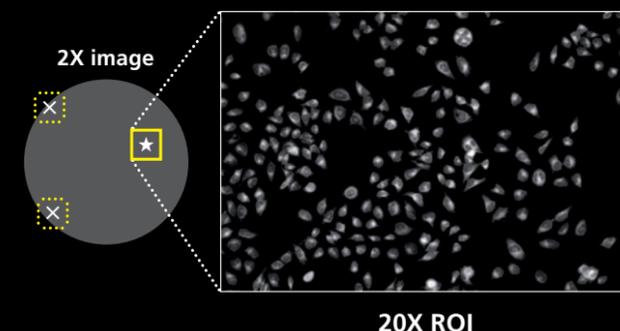

20X ROI

Automatically detect regions with uniform cell density or uniform distribution and then capture image at high-magnification

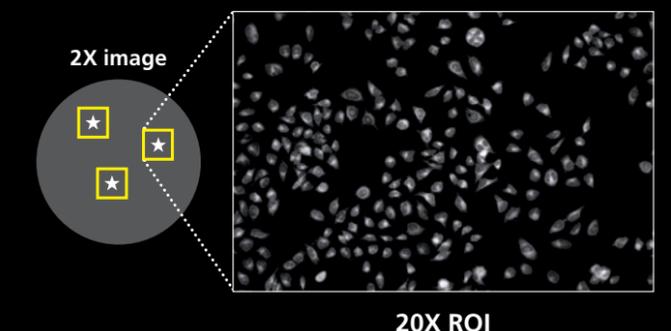

20X ROI




Automatically detect regions that meet conditions input in advance and capture image at high-magnification

# More evolved optical capability that can clearly capture fluorescence samples

## High sensitivity

### Detects even faint fluorescent signals

The Digital Sight 50M achieves quantum efficiency of 85%. Even faint fluorescence signals can be captured by the pixels on account of the broad 3.76 μm pixel pitch and high quantum efficiency.

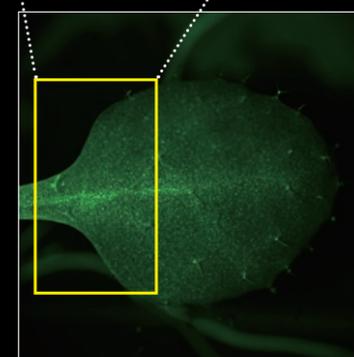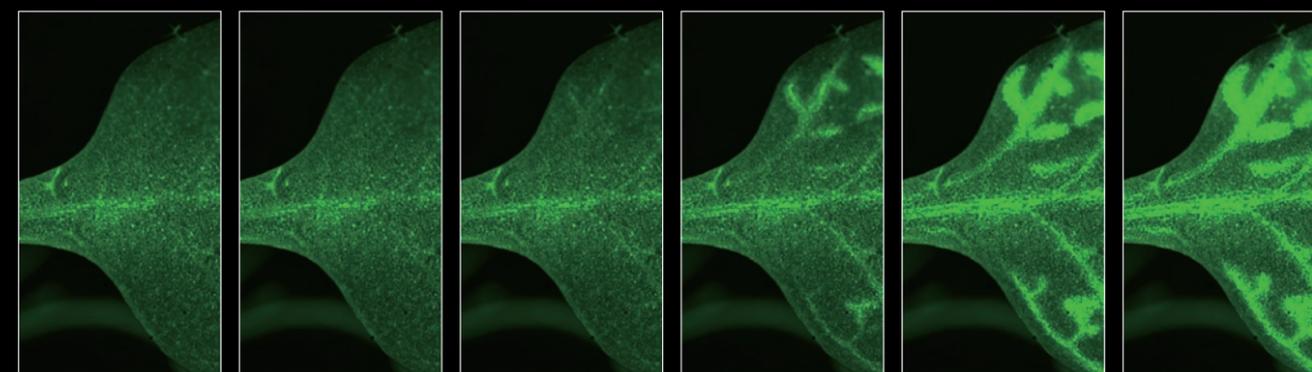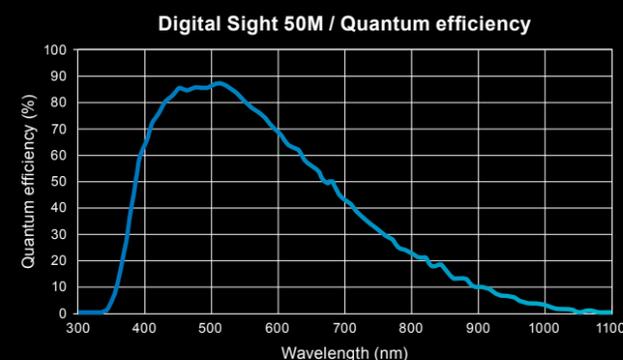


Ca<sup>2+</sup> transfer images of Arabidopsis thaliana with G-Camp  
Interval 1 sec, shooting for 100 sec  
Photo courtesy of : Dr. Masatsugu Toyota, Graduate School of Science & Engineering, Saitama University



## Low noise

### Acquires dim fluorescent signals with ultra-low noise

Both 6e<sup>-</sup> read noise coupled with a large full-well capacity and 1.0e<sup>-</sup>/p/s dark current allow the acquisition of 14bit fluorescence images with very little noise.

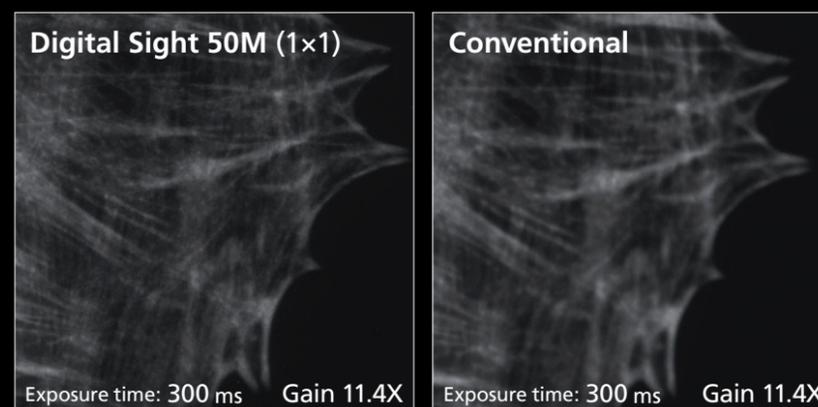

## Time-lapse photography

### Fluorescent time-lapse imaging through integration with NIS-Elements software

With a large field of view and pixel density, and low noise, the Digital Sight 50M is ideal for time-resolved imaging applications.

## Numerous image acquisition modes

### Adjustable balance between quality and speed

There are three operation modes, making it possible to select the required speed and quality. Maximum frame rate of 225.9 fps for high-speed photography.

Mode	ROI size (pixels)	Frame rate	
		8 bits	16 bits
1x1 mode	640x480	113.0 fps	23.6 fps
2x2 mode	640x480	114.9 fps	57.4 fps
3x3 mode	640x480	225.9 fps	112.9 fps

## Fast live display

### Fast focusing, even with fluorescent images

A high-sensitivity CMOS sensor and high-speed data transfer using a general-purpose PC I/F USB 3.2 Gen 1 are combined to achieve 6 fps at the maximum number of pixels (60 megapixels) or a maximum speed of 27 fps (6.7 megapixels). It is also possible to quickly focus on samples.

## 3 types of camera adapters

### Includes 2.5X, 1.8X, and 1X adapters, each for different uses

The Digital Sight 50M offers the large CIS (Nikon FX format) that makes wide field-of-view (FOV25) observations possible.

There are three adapters for different uses: 2.5X and 1.8X adapters for high-resolution single shots of 60 megapixel; and a 1X adapter for samples that require high sensitivity and low noise, such as for image tiling.

For large FOV observations and photography

**2.5X**

Aspect ratio of about 3:2  
ø17.2 mm

High sensitivity observations and photography, for tiling

**1.8X**

Aspect ratio of about 3:2  
ø24 mm

**1X**

Aspect ratio of about 1:1  
ø16,22,25 mm

## ROI mode

### Capture images of regions of the field of view at high speed and in real time

It is possible to freely designate a region and size within the effective pixel scope and then capture images of that desired region at high speed.



## Integration with the comprehensive imaging software series

Nikon uses the NIS-Elements series as control software. NIS-Elements allows functions from basic imaging to control of the microscope and peripheral devices to be performed, as well as the measurement, analysis, and management of acquired images. Four basic packages and a variety of optional modules are available to suit every application and objective.

### F Free package

The bundled free package offers functions for the display of scale on live images, full-screen display, and more. The simple operation screen makes shooting easy.

### D Documentation package

The documentation package is equipped with measurement and report creation functions. It enables general microscopic image acquisition in fields from biomedical to industrial, and is expandable through optional added features such as EDF and databases.

### Br Ar Research package



The research package enables the construction of advanced image acquisition systems, including multidimensional imaging (up to 4 dimensions for Br, 6 dimensions for Ar), through integration with systemized microscopes. Sets equipped with a rich range of image processing and analysis functions are available for every application.

Compatible OS: Windows® 11 Pro (64-bit version)

\* For information about compatible desktop PCs, contact Nikon.


### Multichannel (Multi Color) Ar Br

NIS-Elements can acquire full bit depth multi-color images, combining multiple fluorescence wavelengths and different illumination methods (DIC, phase contrast etc.), while offering independently scalable channels.

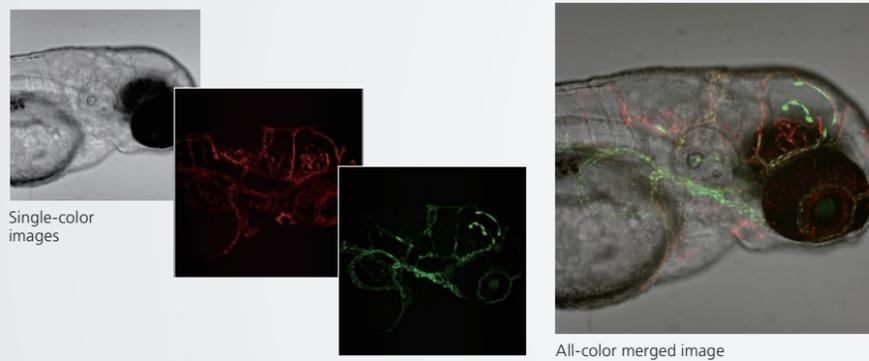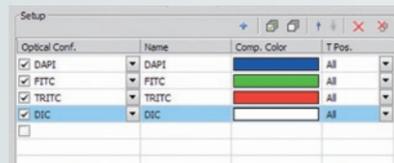


### Z-series Ar Br D

Through motorized focus control, NIS-Elements reconstructs and renders 3D images from multiple Z-axis planes.

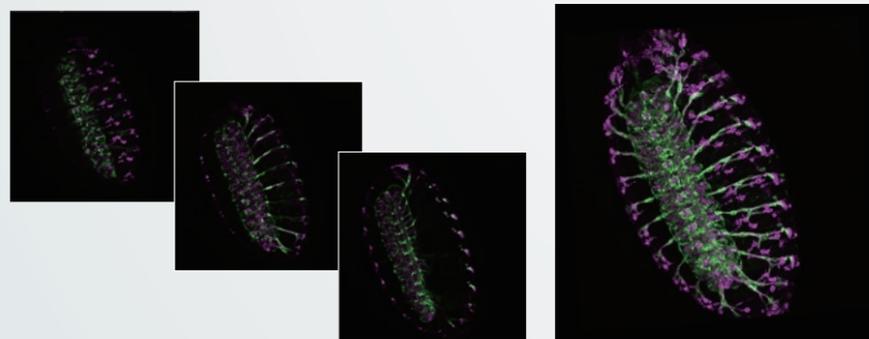


### Multi-dimensional Image Display Ar Br

NIS-Elements displays time lapse, multi-channel, multiple X, Y, Z positions in an intuitive layout, which allows for automatic playback and the ability to select subsections of the data to be saved as a new file.

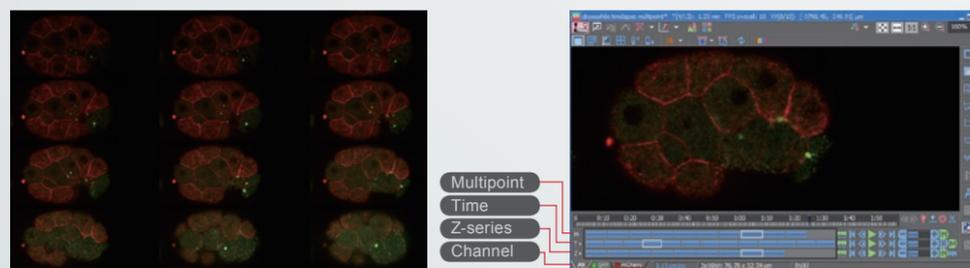

### EDF (Extended Depth of Focus) Option Ar Br D


Creates a single, all-in-focus image from images of differing focus. Such images can now be created by simply turning the focus knob.

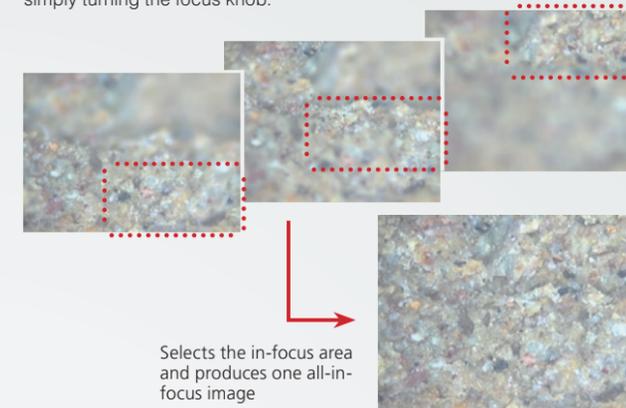

Selects the in-focus area and produces one all-in-focus image


### Image stitching (Large Image) Option Ar Br D

Stitches together images from multiple fields of view during shooting to create an image with wide field of view. Images already acquired can also be stitched together.

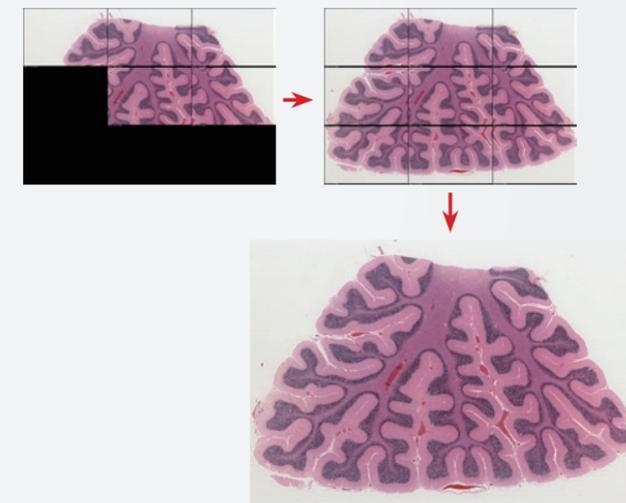


### Manual measurement and image annotation Ar Br D

Manual Measurement allows easy measurement of length and area by drawing lines or an object directly on the image. The results can be attached to the image, and also exported as text or to an Excel spreadsheet.

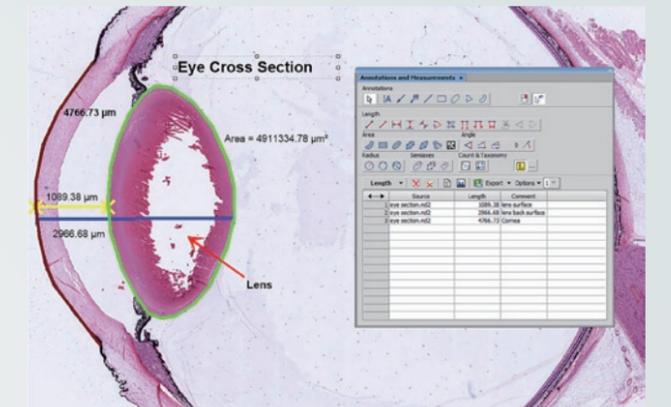

### Auto measurement (Object Counting) Ar Br Option D


Performs binarization on images using previously set thresholds to measure the number, area, brightness, etc. of identified objects.

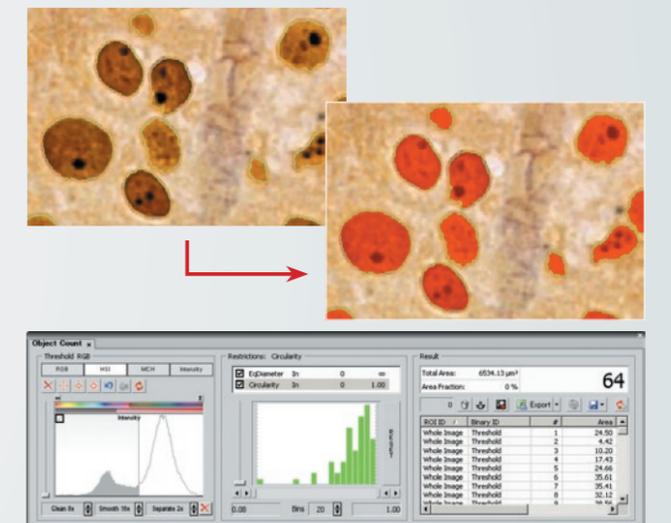

### Classifier


#### Object Classifier Option Ar

Object classifier uses objects identified by thresholding along with additional features such as shape factors, and other statistical methods including nearest neighbor and neural networks for classifying objects into multiple categories. It is also possible to teach the module based on interactive 'picking' of image pixels.

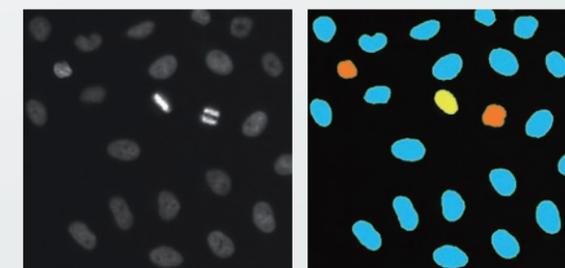

#### Pixel Classifier Ar Br Option D

This function classifies each pixel in the image with RGB/HIS and intensity across the whole image. Results are reported in percentage and it is possible to save and reuse parameters across a large sample of images. Multiple binary layers are also displayed with multiple colors on the image and are available with other analysis tools within the software package.

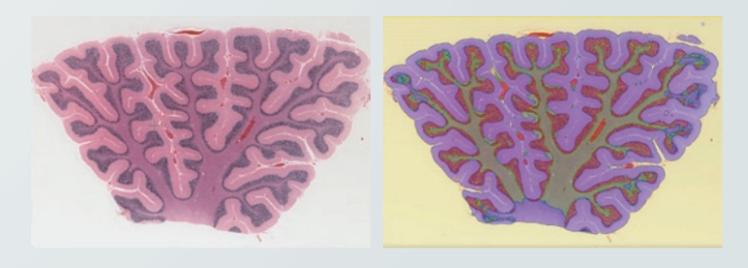




## Allows intuitive control of microscope cameras from tablet PCs

Simply installing NIS-Elements L on a tablet PC enables setting and control of DS-Fi3/Digital Sight 10/Digital Sight 1000 microscope cameras, live image display, and image acquisition.

(Compatible OS: Windows® 11 Pro) \* For information about compatible tablet PCs, contact Nikon.

### User Interface for naturally simple operation

NIS-Elements L displays various menus for image capture, saving, display, measurement and annotations using intuitive icons. It also supports touch screen operation.

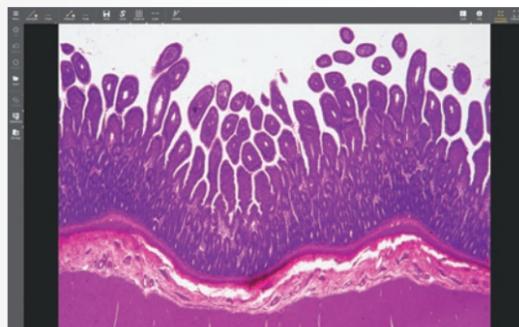

### Scene mode


Ten camera setting patterns for optimal color reproduction and contrast for each microscope light source, observation method and type of sample, as well as custom settings, can be selected. (Available with DS-Fi3/Digital Sight 10/Digital Sight 1000 microscope cameras)

#### Biological Scene Mode

- Brightfield
- HE
- ELISA
- LED-Brightfield
- Asbestos


### A wide variety of tools

NIS-Elements L enables the conducting of simple measurements on images, with input of lines and comments. These can also be written onto and saved with the image, and measurement data can be output.

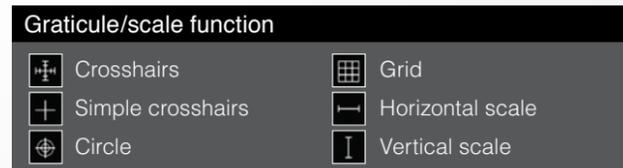

### Other functions


- Split screen display function:** A live image is displayed on the left side of the screen and the saved image is displayed on the right side. When synchronization is activated, synchronized magnification is applied to the both images.
- Camera information:** A histogram and metadata of the image are displayed.
- Full screen:** The image is displayed across the entire screen.
- Saving:** The displayed image is saved with a new file name.

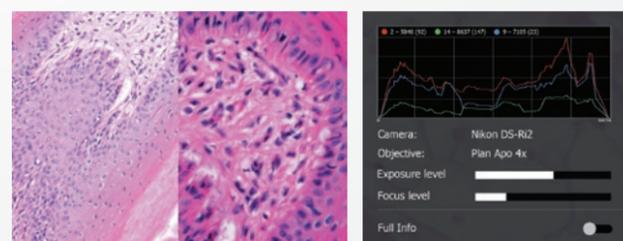

Split screen display function

Camera information

## System Diagram

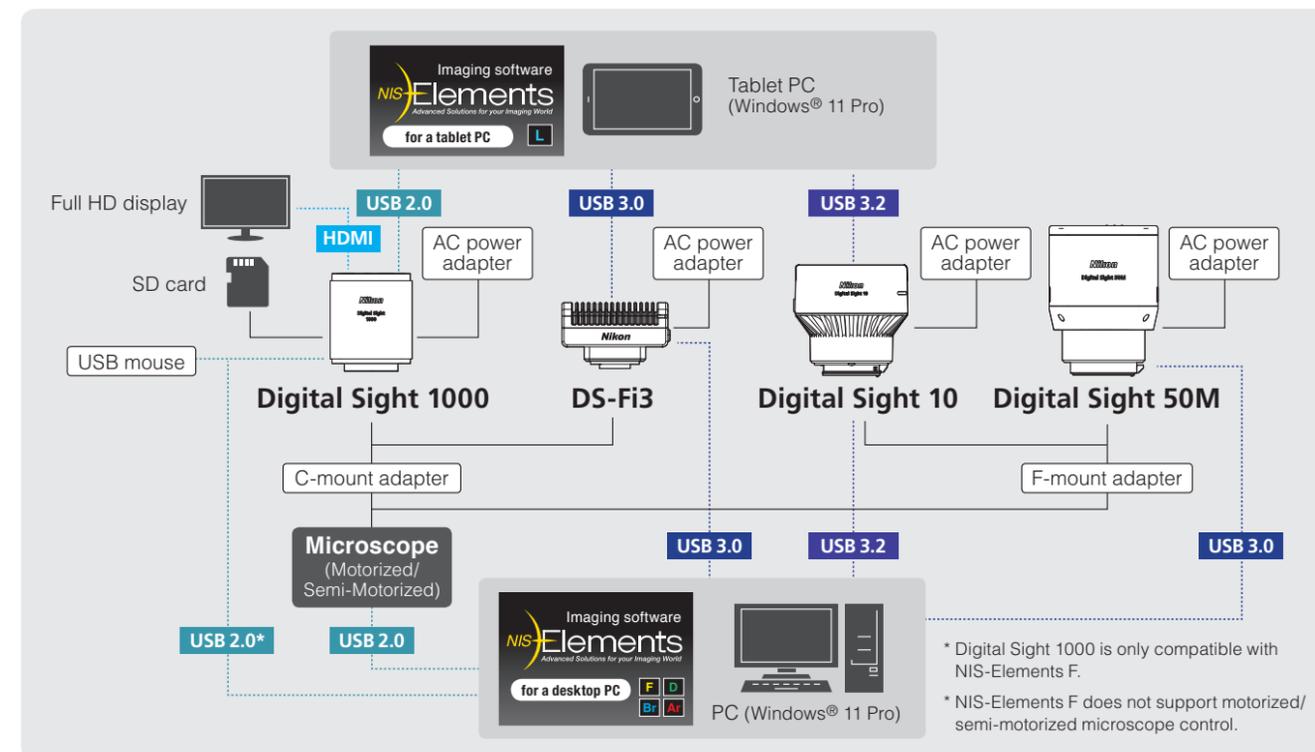

## Specifications


Model name	Digital Sight 1000	DS-Fi3	Digital Sight 10	Digital Sight 50M
Image sensor	1/2.8 inch Color CMOS image sensor Size: 5.57 × 3.13 mm	1/1.8 inch Color CMOS image sensor Size: 6.91 × 4.92 mm	Nikon FX-format Color CMOS image sensor Size: 35.8 × 23.8 mm	Nikon FX-format Monochrome CMOS image sensor Size: 35.8 × 23.8 mm
Recordable pixels	1920 × 1080 pixels	All pixels: 2880 × 2048 2 Vertical and 2 horizontal pixels average: 1440 × 1024	6000 × 3984 pixels	All pixels: 9552 × 6336
Lens mount	C-mount		F-mount	
Cooling method				Electronic cooling
ISO sensitivity (recommended exposure index)	Standard: equivalent to ISO 150	Standard: equivalent to ISO 50 (Selectable from ISO 50 to ISO 3200 equivalent)	Equivalent to ISO 200 (color mode) Equivalent to ISO 800 (monochrome mode) (Selectable from ISO 125 to 8000 :in color / ISO 500 to 32000 in mono)	Equivalent to ISO 200
Quantum efficiency				85 %
Full well Capacity				45000e <sup>-</sup> (typ.)
Readout noise				6e <sup>-</sup>
Dark current				1.0e <sup>-</sup> /p/s (Ta=25°C)(typ.)
Live display mode* (maximum fps)	1920 × 1080 pixels: 30 fps	All pixels (2880 × 2048): 15 fps 2 Vertical and 2 horizontal pixels average (1440 × 1024): 30 fps	All pixels (6000 × 3984): 9 fps FullHD 3x3 pixels average (1920x1080): 66 fps	All pixels (9552 × 6336): 6 fps@8 bit, 1.9 fps@16 bit 3 × 3 pixels average @ 8 bit (ROI 640 × 480): 225.9 fps***
Exposure time	1 m sec–10 sec	100 μsec–30 sec	100 μsec–120 sec	150 μsec–120 sec
Photometry mode	Average photometry 1920 × 1080 pixels (all area)	Average photometry: Average intensity within the photometry area Peak photometry: Maximum intensity within the photometry area		
Exposure control	Automatic exposure, Manual exposure	One-time automatic exposure: Exposure time is adjusted automatically for one-time within the optimum range for the camera Continuous automatic exposure: Automatic exposure adjustment is performed continuously to keep the exposure within the camera Manual exposure: Exposure time and gain settings are made manually		
Exposure correction	Available	Average metering: ±1EV Step:1/6EV (some restrictions according to tone) Peak hold metering: -1 EV ~ ±0 EV		Average metering: -1 EV ~ +1/2 EV Peak hold metering: -1 EV ~ ±0 EV
Interface	USB2.0 (connect with PC or USB mouse) × 1, HDMI × 1, SD card slot x1**	USB3.0 (connect with PC) × 1, External trigger × 1	USB3.2GEN1,2 (connect with PC) × 1, External trigger × 1	USB 3.2GEN1 (connect with PC) × 1, External trigger × 1
Power supply	AC100-240V 50Hz/60Hz			
Power consumption	3 W	4.8 W	18 W	27 W
Operating environment	0-40°C, 60% RH max. (without condensation)			

\*Maximum frame rate depends on exposure time. \*\*Both SD and SDHC memory cards are available.

\*\*\*When using NIS-Elements, 16-bit mode can be selected for 1x1 and 2x2 digital binning, and 12-bit mode can be selected for 2x2, 3x3, 4x4 and 6x6. 8-bit mode can be selected in all image size modes.


# Dimensions

## Digital Sight 1000

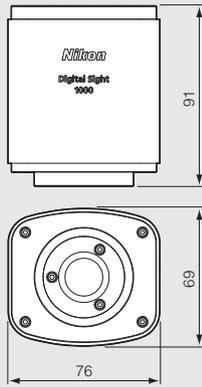


Weight: approx. 450 g

## DS-Fi3

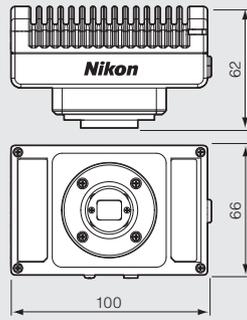

Weight: approx. 400 g

## Digital Sight 10

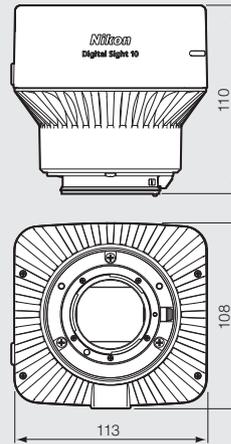


Weight: approx. 1,100 g



Digital Sight 10  
Maintenance movie

## Digital Sight 50M

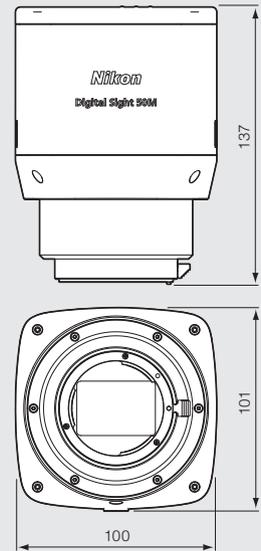

Weight: approx. 1,300 g

The digital sight series is not for clinical diagnostic use.

Specifications and equipment are subject to change without any notice or obligation on the part of the manufacturer. October 2024 ©2004-2024 NIKON CORPORATION  
Microsoft and Windows are registered trademarks of Microsoft Corporation in the United States and other countries. Company and product names listed in this catalog are trademarks or registered trademarks of each company.

N.B. Export of the products\* in this catalog is controlled under the Japanese Foreign Exchange and Foreign Trade Law.  
Appropriate export procedures shall be required in case of export from Japan.

\*Products: Hardware and its technical information (including software)



**WARNING** TO ENSURE CORRECT USAGE, READ THE CORRESPONDING MANUALS CAREFULLY BEFORE USING THE EQUIPMENT.



### NIKON CORPORATION

Head office  
1-5-20, Nishi-cho, Shinagawa-ku, Tokyo, 140-8601, Japan  
<https://www.healthcare.nikon.com/en/>

### Manufacturer

471, Nagaodai-cho, Sakae-ku, Yokohama,  
Kanagawa 244-8533, Japan

ISO 14001 Certified  
for NIKON CORPORATION

### Nikon Instruments Inc.

1300 Walt Whitman Road, Melville, N.Y. 11747-3064, U.S.A.  
phone: +1-631-547-8500; +1-800-52-NIKON (within the U.S.A. only)  
fax: +1-631-547-0299  
<https://www.microscope.healthcare.nikon.com/>

### Nikon Europe B.V.

Stroombaan 14, 1181 VX Amstelveen, The Netherlands  
phone: +31-20-7099-000  
[https://www.microscope.healthcare.nikon.com/en\\_EU/](https://www.microscope.healthcare.nikon.com/en_EU/)

### Nikon Precision (Shanghai) Co., Ltd.

CHINA phone: +86-21-6841-2050 fax: +86-21-6841-2060  
(Beijing branch) phone: +86-10-5831-2028 fax: +86-10-5831-2026  
(Guangzhou branch) phone: +86-2-3882-0551 fax: +86-2-3882-0580  
<https://www.nikon-precision.com.cn/>

### Nikon Canada Inc.

CANADA phone: +1-905-625-9910 fax: +1-905-602-9953

### Nikon France, Succursale de Nikon Europe B.V.

FRANCE phone: +33-1-4516-4516

### Nikon Deutschland, Zweigniederlassung der

### Nikon Europe B.V.

GERMANY phone: +49-211-9414-888

### Nikon Italy, Branch of Nikon Europe B.V.

ITALY phone: +39-055-300-9601

### Nikon Europe B.V., Amstelveen,

### Zweigniederlassung Schweiz (Egg/ZH)

SWITZERLAND phone: +41-43-277-2867

### NIKON UK, Branch of Nikon Europe B.V.

UNITED KINGDOM phone: +44-208-247-1717

### Nikon Österreich, Zweigniederlassung der

### Nikon Europe B.V.

AUSTRIA phone: +43-1-972-6111

### Nikon Singapore Pte Ltd

SINGAPORE phone: +65-6559-3651 fax: +65-6559-3668

### Nikon Australia Pty Ltd

AUSTRALIA phone: +61-2-8767-6900

### Nikon Instruments Korea Co., Ltd.

KOREA phone: +82-2-6288-1900 fax: +82-2-555-4415

### NIKON INDIA PVT. LTD.

AUSTRALIA phone: +91-124-4688-500

Code No. 2CE-MPAK-6 (2410) Am