




Mitutoyo

Hardness Testing Machines **HM-200 Series**

TEST EQUIPMENT AND
SEISMOMETERS

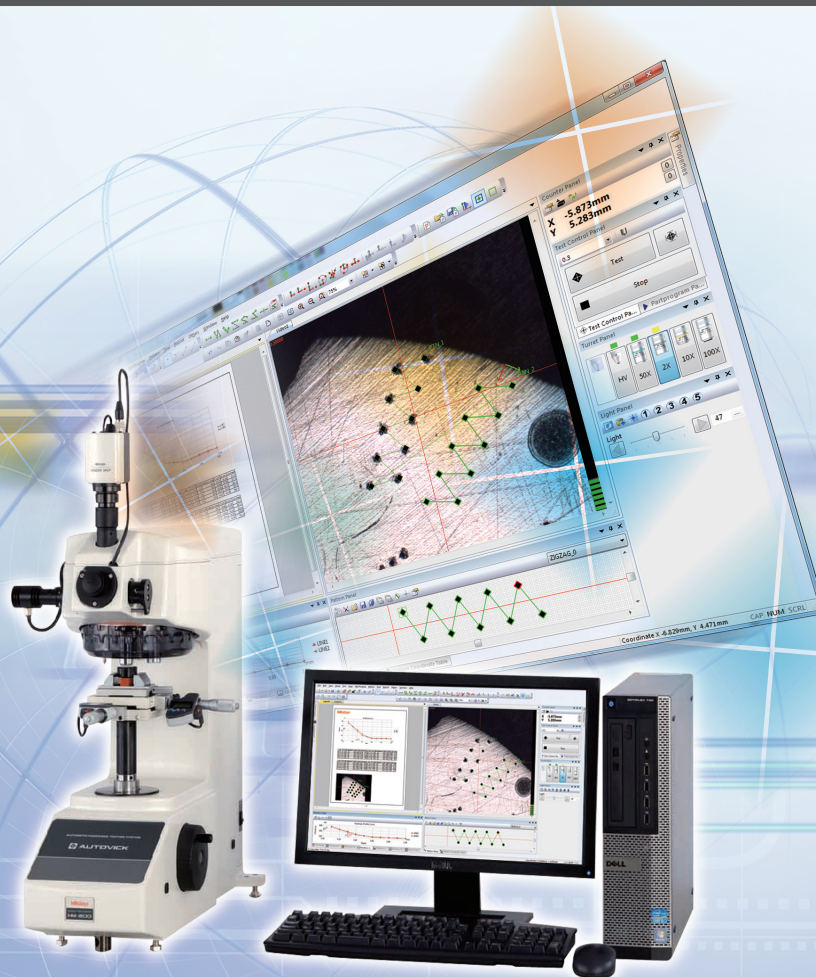

Micro Vickers Hardness Testing Machines HM-200 Series

Equipped with the latest optical system
ideal for measuring the dimensions of indentation
and a test-force loading device that lets you set the
The HM-200 series is ideal for quality control
and mechanical characteristic evaluation using
Vickers hardness testing of small areas.



Features

- Touch-panel operation
- Measurement of indentation dimensions using a measuring microscope
- Positioning using a manual XY stage unit



Images
desired test force!

Automatic dimensions by AVPAK eliminates indentation measurement errors.





B

HM-210B•HM-220B

Features

- Operation using AVPAK
- Automatic measurement of indentations
- Positioning using a manual XY stage

Functions	System A	System B
		
Focusing	Manual	Manual
Testing action	Single point	Single point
Test-point positioning	Manual XY stage	Manual XY stage
Measuring indentations	Measuring microscope	Automatic (AVPAK)
Camera (for observing and measuring indentations)	Monochrome, 300,000 pixels*	Color, 3 million pixels
Operating the main unit	Touch panel	PC (AVPAK)

*When a video camera unit is used (pixel count of the camera itself: 380,000)



HM-210/220 Manual model main unit

High-functionality model for Systems A

Measuring microscope

Microscope for measuring indentation dimensions.
Integrated 10X eyepiece.
(810-354 video camera unit can be installed)

New

LED illumination unit

Uses an LED illumination unit that offers a long service life and low power consumption.
LED illumination reduces the time lost during the light bulb replacement required with conventional illumination units.

Automatic turret mechanism

The positions of the indenter and the objective lens can be automatically switched using touch panel operation (can also be manually switched).
Up to four objective lenses can be installed.
Up to two indenter shaft units can be installed.

Wide range of test force

Use of an electromagnetic method makes it possible to set the desired test force, between 0.4903 mN and 19610 mN. (HM-220)

New

Objective lenses provide a long working distance

Six MH Plan objectives are available. The 10X, 20X, 50X, and 100X types are used when measuring indentations, and the 2X and 5X for widefield observation tasks.

Manual XY stage unit with digital micrometer head

During test-site positioning, the positional information is displayed digitally and can also be displayed on the touch panel display controller.
25 × 25 mm or 50 × 50 mm stroke can be selected.

Color touch panel controller

Touch panel operations for controlling hardness testing provide a full suite of basic functions necessary for hardness testing, a function for converting the hardness value into various types of hardness scales, and a statistical calculation function.

Interfacing to external instruments

Provided with a wide variety of interfaces to suit any purpose.
Test results can be printed on a printer or output to a PC.

- USB 2.0 interface (for data communication)
For PC (EXPAK ver6)
- Digimatic interface
For DP-1VR, U-WAVE, and USB-ITN
- Serial interface
For DPU-414

Video camera unit 810-354

(Can be installed in the manual model main unit)

CCD camera and 8.4-inch TFT monitor.
Enables observation and measurement of indentations at high magnification, thereby reducing operator error.





HM-210/220 System model main unit

High-functionality model for Systems B

Measuring microscope (Can be installed as an option)

Enables magnified observation and measurement of indentations.
(The vision unit integrated in the system model main unit and the measuring microscope cannot be simultaneously used for observation.)

New

LED illumination unit

Uses an LED illumination unit that offers a long service life and low power consumption.
LED illumination reduces the time lost during the light bulb replacement required with conventional illumination units.

Automatic turret mechanism

The positions of the indenter and the objective lens can be automatically switched from a PC (AVPAK) (can also be manually switched). Up to four objective lenses can be installed.
Up to two indenter shaft units can be installed.

New

Vision unit

USB color mega-pixel camera
A 3-million pixel, 1/2-inch color USB camera is used for the system model.

Wide range of test force

Use of an electromagnetic method makes it possible to set the desired test force very accurately, between 0.4903 mN and 19610 mN. (HM-220)

New

Objective lenses provide a long working distance

Six MH Plan objectives are available. The 10X, 20X, 50X, and 100X types are used when measuring indentations, and the 2X and 5X for widefield observation tasks.
2X and 5X for wide-field observation.

Manual XY stage unit with digital micrometer head (System B)

During test-site positioning, the positional information is displayed digitally.
25 × 25 mm or 50 × 50 mm stroke can be selected.

connection



AVPAK software for automatic hardness testing systems

Software that supports control, testing, and report creation related to hardness testing.
Supports parameter setting and automatic measurement.

High-functionality PC and TFT monitor

Compatible with Windows 7 Professional 32-bit.
Supports a wide-screen TFT and provides improved operability.


New

HM-200 Series AVPAK software for controlling Systems B

Screen layout for control, testing status, and result display can be changed freely.

Graphic view (of stored images)

For displaying the entire specimen and checking the pattern positioning. The digital zoom function can be used to easily magnify and check the site being tested.




Layout view

Photos from individual views, graphs, tables, etc., can be laid out freely to help with report creation.


Part program

Automatically records the sequence of operations in a test. To repeat the same test, the part program can be called up for repeated execution.

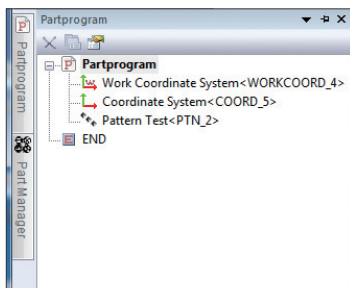


Part manager

Test result view

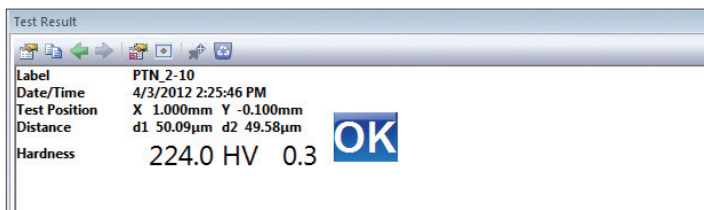


Pattern creation

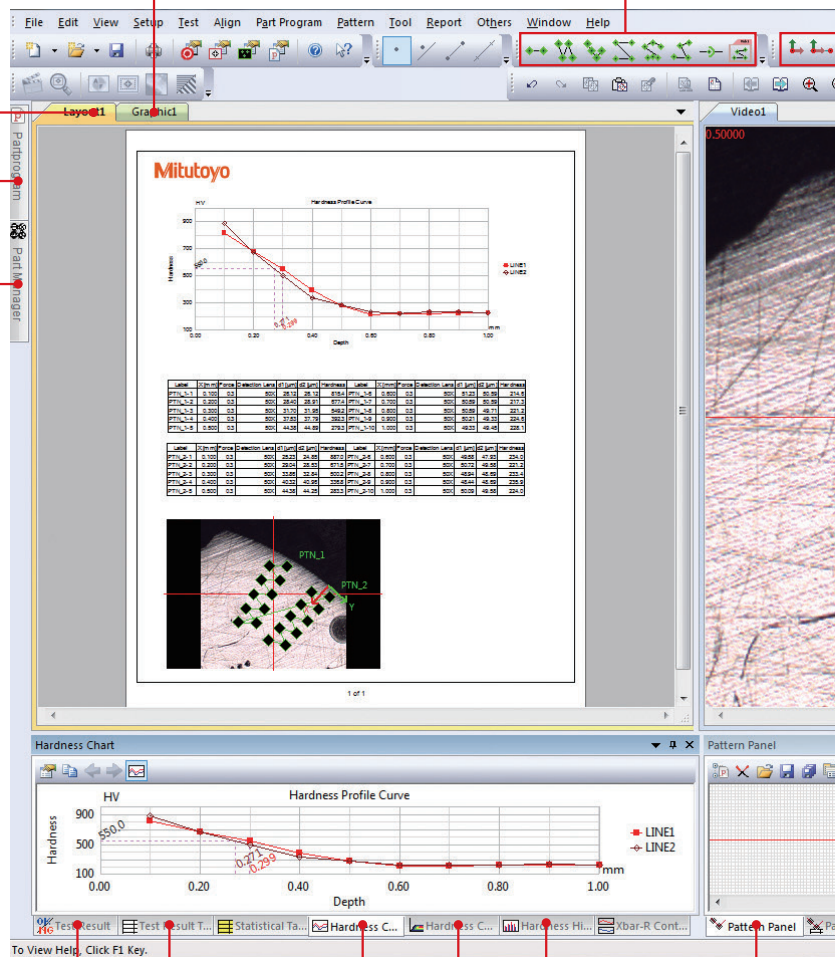

Test result list view

Hardness curve graph

Hardness distribution diagram

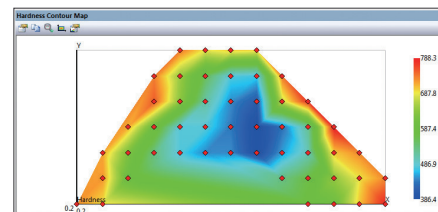



Pattern pasting

Video view (live image)
Indentation image display
Small indentations can be observed using the digital zoom function.

Contrast level meter
Stable focusing can be easily achieved by anyone.

Counter
Displays the stage's current coordinates.

Properties panel


Test control
Controls testing actions such as wide- or narrow-range auto-focusing and measurement of indentations.

Turret control
Switches the objective lens and indenter shaft.



Illumination control
Controls the illumination in 100 steps.

Indentation-reading example

Pattern panel

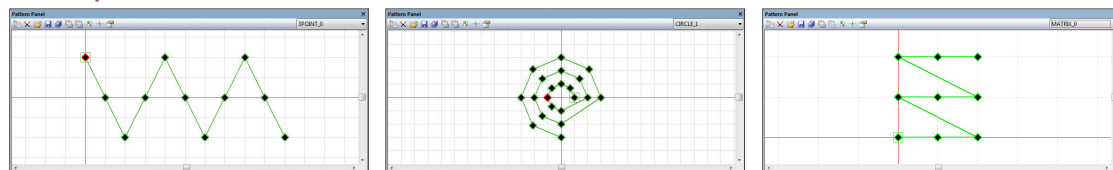


Frequency distribution graph

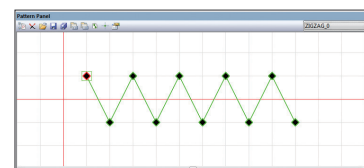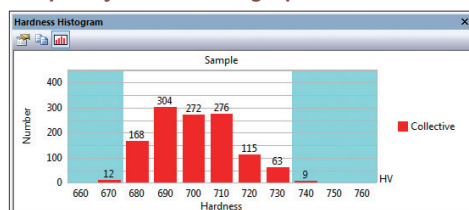

HM-200 Series AVPAK software for controlling Systems B

New functions



Pattern creation

This tool supports the creation of test patterns such as straight lines, zigzag lines, and teaching patterns.



Pattern pasting

This tool supports the pasting of created test patterns. It adjusts the origin, direction, etc., to paste a pattern.

Handling of multiple specimens

Multiple specimens can be tested when a part program and Parts Manager are used.

Parts Manager


Executes a common part program for specimens having the same shape.



Reading of indentations



Improvement in image-processing performance has improved the indentation measurement function.

*measurement accuracy varies according to conditions.

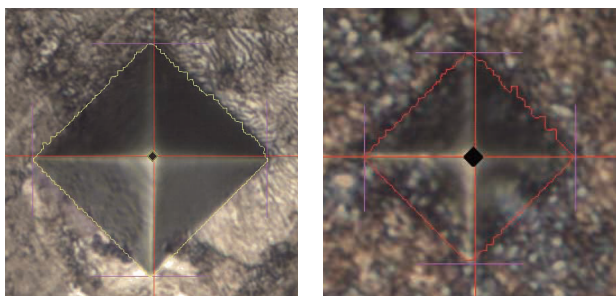



Indentation depth display

Displays the indentation depth of the diamond indenter while the testing force is being applied. (Reference value)





Property panel

Used for setting the test conditions such as the test force and load time, as well as the indentation measurement condition.



Navigation function

When the test position is being moved during multi-point testing, this function guides the travel of the XY fine adjustment manual stage to the next position.




HM-200 Series


Touch-panel control screen & System outline drawing

Touch-panel control screen


Easy-to-understand graphic display enables intuitive operation. Functions for converting values and compensating for curved surfaces, as well as a test condition guiding function are all provided as standard features.
(Installed in the manual model main unit)

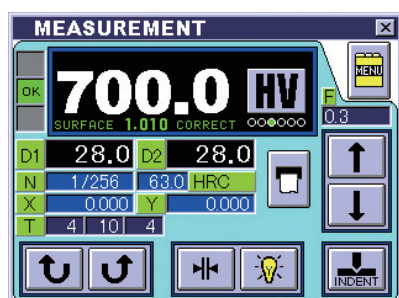


Displays test conditions and test results.

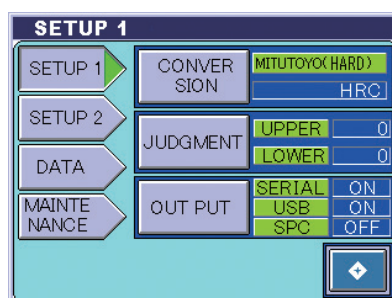


Used for selecting a conversion scale, entering a setting for Pass/Fail determination, and specifying external output.

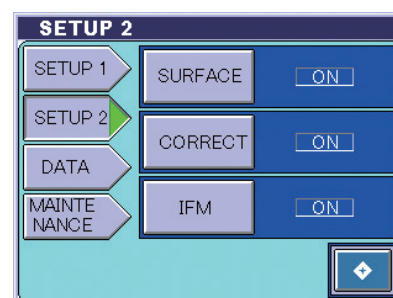


Used for selecting a conversion scale, entering a setting for Pass/Fail determination, and specifying external output.

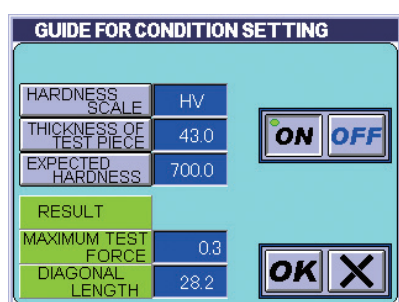

By entering the specimen thickness and the presumed hardness, you can set a test force that satisfies the JIS conditions.

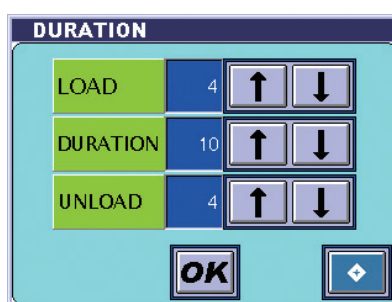


In addition to the test force dwell time, you can specify loading and unloading testing actions.

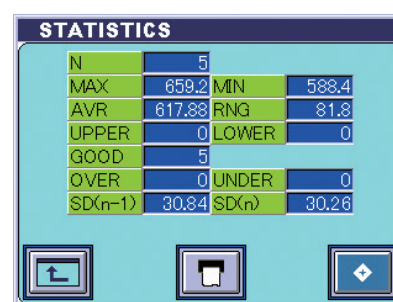


You can check the test results in a statistical list.

System A Outline drawing

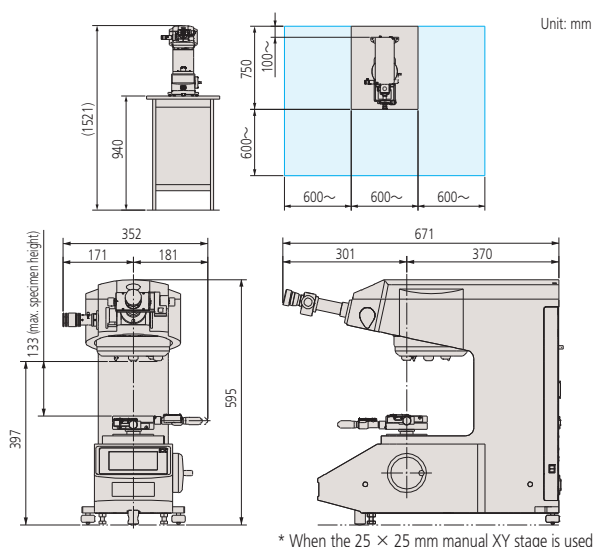

System B Outline drawing

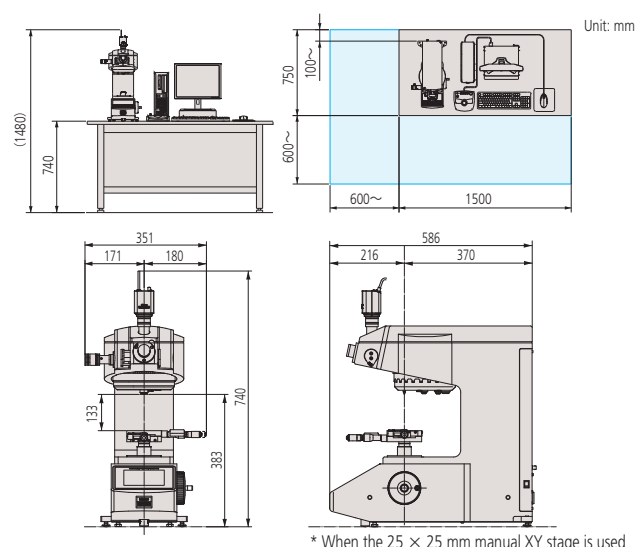

System configurations

	Code No.	Item name	System A	System B	Details	Notes
Main unit	810-400*	HM-210 manual model main unit	○	×	Standard test force, measuring microscope, with a 50X lens	
	810-405*	HM-220 manual model main unit	○	×	Low test force, measuring microscope, with a 50X lens	
	810-403*	HM-210 system model main unit	×	○	Standard test force, with a 50X lens	No measuring microscope, No touch panel
	810-408*	HM-220 system model main unit	×	○	Low test force, with a 50X lens	
	11AAC104	Objective lens unit 2X	○		Objective lens, with lens holder	Up to three additional lenses can be selected (maximum of four lenses can be installed in the main unit)
	11AAC105	Objective lens unit 5X	○		Objective lens, with lens holder	
	11AAC106	Objective lens unit 10X	○		Objective lens, with lens holder	
	11AAC107	Objective lens unit 20X	○		Objective lens, with lens holder	
	11AAC108	Objective lens unit 100X	○		Objective lens, with lens holder	
	11AAC109	Indenter shaft unit for HM-210	○		With 19BAA061 knoop indenter	Double-indenter specification
	11AAC110	Indenter shaft unit for HM-220	○		With 19BAA062 knoop indenter	Double-indenter specification
	11AAC129	Measuring microscope (which can be added)	×	○		Cannot be used simultaneously with the VISION UNIT
	810-354*	Video camera unit	○	△	Monochrome 300,000-pixel camera, 8.4-inch TFT, with a stand	△: Installation requires a measuring microscope. Provided on a special order basis
Essential options	810-420	Manual XY stage unit 25X25	☆	☆		
	810-423	Manual XY stage unit 50X50				
	810-424	Manual XY stage unit 1"x1"				
	810-427	Manual XY stage unit 2"x2"				
	11AAC316	AVPAK-20	×	☆		Selected according to the delivery destination
Special accessories	810-016	Standard vise	○		Jaw opening: 51 mm	
	810-017	Special vise	○		Jaw opening: 100 mm	
	810-013	Thin plate specimen holder	○		Thickness: Max. 5 mm	
	810-014	Slender specimen holder (horizontal)	○		Diameter: 0.4-3 mm	
	810-015	Slender specimen holder (vertical)	○		Diameter: 0.4-4 mm	
	810-019	Specimen-tilting holder	○		Jaw opening: 37 mm, Tilting angle: ±15°, Rotating angle: ±25°	
	810-020	Universal specimen holder	○		Thickness: Max. 30 mm	
	810-018	Turntable	○		Minimum graduation: 1°	
	810-085	Adjustable thin-plate specimen holder	○		Thickness: Max. 3 mm, Width: Max. 56 mm	
	810-095	Rotatable tilting specimen holder	○		Height: Min. 20 mm, Width and diameter: 15-55 mm	
	810-870*	Specimen heater HST-250	○	△		△: Cannot be automatically read with AVPAK
	810-650-1	Resin-molded specimen holder Ø25.4	○		Ø25.4±0.5 mm Specimen height: 9-39 mm	
	810-650-2	Resin-molded specimen holder Ø30	○		Ø30±0.5 mm Specimen height: 9-39 mm	
	810-650-3	Resin-molded specimen holder Ø31.75	○		Ø31.75±0.5 mm Specimen height: 9-39 mm	
	810-650-4	Resin-molded specimen holder Ø38.1	○		Ø38.1±0.5 mm Specimen height: 9-39 mm	
	810-650-5	Resin-molded specimen holder Ø40	○		Ø40±0.5 mm Specimen height: 9-39 mm	
	19BAA061	Knoop indenter (for standard test force)	○			Can be selected to replace the Vickers indenter provided as a standard accessory.
	19BAA062	Knoop indenter (for low test force)	○			
	375-056	Objective micrometer	×	○	Scale graduation: 1 mm, Minimum graduation: 0.01 mm	For magnification calibration
Printers	02AGD600*	Model DPU-414 (with a connection cable)	○	×	Receipt printer	For 100V
	264-504*	Model DP-1VR	○	×	Digimatic mini-processor	
	936937	Connection cord	○	×	For DP-1VR 1 m	
	02AZD810D	U-WAVE-R	○	×		
	02AZD880D	U-WAVE-T	○	×	Buzzer type	
	02AZD790D	Dedicated connection cable for U-WAVE-T	○	×		
	06ADV380D	USB-ITN-D	○	×	Flat 10-pin	PC must be provided separately.
	—	EXPAK ver6	○	×		Requires Microsoft Excel 2010
Others	02ATE760	Table	○		1800 (W) x900 (D) x740 (H)	For tester and PC
	998923	System rack (vertical)	○			Only a PC can be mounted.
	810-641	Vibration isolator	○			Only the tester can be mounted.
	810-644	Wing for vibration isolator	○		For 810-641	Recommended if the video camera unit is to be attached
	11AAC146	Plate for preventing toppling	○			

○: Selectable ☆: One of each type must be selected from the choice offered ×: Cannot be selected △: Contact Mitutoyo Sales Dept.
Note: A suffix replaces the * symbol.



Specifications Main Unit

Model name			HM-210A					HM-210B				
Main unit	HM-210 manual model main unit	810-401*	○					—				
	HM-210 system model main unit	810-403*	—					○				
Hardness tester	Applicable standards		JIS B 7725 / ISO 6507-2									
	Test force		Hardness symbol	HV0.01	HV0.02	HV0.03	HV0.05	HV0.1	HV0.2	HV0.3	HV0.5	HV1
			N	98.07x10 ⁻³	196.1x10 ⁻³	294.2x10 ⁻³	490.3x10 ⁻³	980.7x10 ⁻³	1.961	2.942	4.903	9.807
			(gf)	(10)	(20)	(30)	(50)	(100)	(200)	(300)	(500)	(1000)
	Indenter approach speed		Fixed at 60 μm/s									
	Test force loading time		1- 99s Can be set in 1s increments.									
	Test force dwell time		0-999s Can be set in 1s increments.									
	Test force unloading time		1- 99s Can be set in 1s increments.									

Model name			HM-220A					HM-220B				
Main unit	HM-220 manual model main unit	810-405	○					—				
	HM-220 system model main unit	810-408	—					○				
Hardness tester	Applicable standards		JIS B 7725 / ISO 6507-2									
	Test force											
	Hardness symbol	HV0.0005	HV0.001	HV0.002	HV0.003	HV0.005	HV0.01	HV0.02	HV0.03	HV0.05	HV0.1	
	N	0.4903x10 ⁻³	0.9807x10 ⁻³	1.961x10 ⁻³	2.942x10 ⁻³	4.903x10 ⁻³	9.807x10 ⁻³	19.61x10 ⁻³	29.42x10 ⁻³	49.03x10 ⁻³	98.07x10 ⁻³	
	(gf)	(0.05)	(0.1)	(0.2)	(0.3)	(0.5)	(1)	(2)	(3)	(5)	(10)	
	Hardness symbol	HV0.02	HV0.03	HV0.05	HV0.1	HV0.2	HV0.3	HV0.5	HV1	HV2		
	N	196.1x10 ⁻³	294.2x10 ⁻³	490.3x10 ⁻³	980.7x10 ⁻³	1.961	2.942	4.903	9.807	19.61		
	(gf)	(20)	(30)	(50)	(100)	(200)	(300)	(500)	(1000)	(2000)		
Indenter approach speed			Variable between 2 and 60 μm/s Can be set in 1 μm/s increments (only for 30 gf or smaller; Fixed at 60 μm/s for 31 gf or greater)									
Test force loading time			1- 99s Can be set in 1s increments.									
Test force dwell time			0-999s Can be set in 1s increments.									
Test force unloading time			1- 99s Can be set in 1s increments.									

Mechanism	Loading device	Test force control	Electromagnetic (voice coil)		
		Test force switching	Can be selected from touch panel		
	Turret	Drive method	Motor drive		
		Operation method	Touch panel / Manual	AVPAK / Manual	
		Number of turret ports	Indenter shaft unit: Up to two can be installed (including the standard Vickers indenter shaft unit already installed); Objective lens unit: Up to four can be installed (including the standard 50X objective lens already installed)		
Controller	Display content	Integrated touch panel (5.7-inch color LCD)		Data-processing software Software (AVPAK) functions <ul style="list-style-type: none">• Tester and turret control functions• Hardness conversion, compensation for curved surface, Pass/Fail determination, and statistical calculation• measurement of indentations, illumination control• Contrast level meter• Specification of test pattern and coordinate system• Simple operations• Analysis and report	
		Indentation value	D1 D2, max. 5 digits each		
		Minimum display unit	For objective lenses of 50X or higher: 0.01 μm; For lower than 50X: 0.1 μm		
		Hardness value	Maximum of four digits, Minimum: 0.1 HV/HK, Fracture toughness value		
		Test condition	Indenter (HV/HK), test force, loading, dwell, and unloading times		
		Compensation	Cylinder, sphere, measurement		
		Pass/Fail determination	OK/±NG		
		Other	XY positional data, turret position display, statistical calculation		
	Calculation functions	Language used	Japanese, English, German, French, Italian, Spanish		
		Pass/Fail determination function	Determines whether or not the measured hardness is acceptable (OK/±NG) based on the upper and lower limits that have been set.		
		Function for guiding measurement condition setup	Enter the indenter, specimen thickness, and presumed hardness to calculate the maximum test force.		
		Compensation function	Cylindrical compensation, spherical compensation, measurement compensation		
		Statistical calculation function	Number of data units, maximum value, minimum value, average, range, upper limit, lower limit, number of passes, number of fails, ultra upper limit and ultra lower limit, standard deviation (n-1), standard deviation (n)		
External connection interface		For printer: Serial interface (compatible with the RS-232C standard); For Digimatic interface and data communication: USB 2.0			
	Maximum specimen dimensions	Maximum specimen depth: 160 mm, Maximum specimen height: 133 mm			
	Maximum load capacity	3kg			
Main unit	External dimensions (excluding protrusions and stage)	Approx. 315 (W) x 671 (D) 595 (H) mm		Approx. 315 (W) x 586 (D) 741 (H) mm	
	Main unit mass	Approx. 43 kg			
Main unit power supply		39VA AC100V: AC100-125V, AC200V: AC220-240V			

Note: A suffix replaces the * symbol.

Specifications Optical system

Item name		HM-210 manual model main unit	HM-220 manual model main unit	HM-210 system model main unit	HM-220 system model main unit
Optical system		Infinitely corrected optical system, 4-port objective lens switching method			
Tube lens magnification		1x			
Illumination	Light source	White LED			
	Aperture diaphragm	Variable			
Standard objective lens	Lens	MH Plan 50x			
	Working distance [mm]	2.5			
	Real field of view and imaging range	Real field of view: ø0.14 mm		Imaging range: 0.118 (H) mm x 0.089 (V) mm	
Measuring microscope (Ocular)		Length-measuring microscope with integrated encoder and eyepiece (10X)		Factory-installed options	
Objective lens unit (including holder) (factory-installed options)		MH Plan 2x	MH Plan 5x	MH Plan 10x	MH Plan 20x
Part No.		11AAC104	11AAC105	11AAC106	11AAC107
Working distance [mm]		6	27	11.8	5.2
Measurement range [Ø mm]		3.5 (reference)	1.4 (reference)	0.7	0.35
Imaging range [(H) mm x 0.089 (V) mm] (Vision unit)		2.95x2.21	1.18x0.89	0.59x0.44	0.30x0.22
					0.059x0.044



■ Specifications Manual XY stage unit

Systems A and B

Item name	Manual XY stage unit 1"x1"	Manual XY stage unit 2"x2"	Manual XY stage 25X25	Manual XY stage 50X50
Code No.	810-424	810-427	810-420	810-423
Stage travel range	25.4×25.4mm	50.8×50.8mm	25×25mm	50×50mm
Table size	100×100mm	130×130mm	100×100mm	130×130mm
Minimum display unit	0.001mm/0.0005"		0.001mm	
XY stage dimensions	221(W)×221(D)×37(H)mm	305(W)×305(D)×49(H)mm	221(W)×221(D)×37(H)mm	305(W)×305(D)×49(H)mm
XY stage mass	2.5kg	6.6kg	2.5kg	6.6kg

■ Standard accessories

Code No.	Item name	Specification/Remarks	Quantity
19BAA058	Diamond indenter*1	Vickers for HM-210	1
19BAA059	Diamond indenter*1	Vickers for HM-220	
—	Hardness testing block*2	700HVM0.3 25 mm (diameter) × 6 mm (thickness)	1
—	Indenter shaft unit*1	With Vickers indenter	1
—	Objective lens unit 50X*1		1
19BAA133	Spacer	Material: Bakelite 11 (W) × 42 (D) × 13 (H) mm	1
11AAB405	Extension shaft	For elevation shaft: 38 mm With two set screws	1
11AAB406	Extension shaft	For elevation shaft: 76 mm With two set screws	1
02DEA471	Dust cover	For the hardness tester main unit	1
—	Plastic Phillips screwdriver	No.1300 Phillips 2×100	1
—	Precision flathead screwdriver	No.205 flathead 1.2	1
—	Hex-head screwdriver	1.5 mm	1
—	Hex-head screwdriver	2.5 mm	2
—	Hex wrench	2.5 mm	1
—	Hex wrench	3.0 mm	1
—	Holder	Hanger bolt for the main unit	4
—	Cap*1	Cap for the holder	4
—	Cable clamp	Gray	2
—	Cable clamp	Black	2
—	Spiral tube	Black, approx. 2 m	1
02ZAA000	Power supply cord set -PSE	Classification: Unmarked/C	1 Depends on the delivery destination
02ZAA010	AC cord set-UL/CSA	Classification: A	
02ZAA020	AC cord set-UL/CSA	Classification: D	
02ZAA030	AC cord set-UL/CSA	Classification: E	
02ZAA040	AC cord set-UL/CSA	Classification: DC	
02ZAA050	AC cord set-UL/CSA	Classification: K	1 Depends on the delivery destination
99MBG127J	User's manual for the manual model main unit	Japanese	
99MBG127A	User's manual for the manual model main unit	English	
99MBG137J	User's manual for the system model main unit	Japanese	
99MBG137A	User's manual for the system model main unit	English	
11AAC198	Configuration disk	For the system main unit	1 Depends on the model
11PAA074	Accessory case		1
—	Certificate for the tester	In both Japanese and English	1
—	Certificate for the hardness test block	In both Japanese and English	1
—	Warranty	In both Japanese and English	1
—	USB camera (system main unit)*1	3 million pixels, 1/2-inch color Systems B	1

*1 Already installed in the main unit when it is delivered.

*2 The numeric values shown are nominal; actual values will be slightly above or below the nominal values.

Specifications are subject to change without notice.

■ Specifications Video camera unit

System A

Item	Description
TFT screen magnification	10X: Approx. 200 times (approx. 260 times) 50X: Approx. 1000 times (approx. 1300 times) 100X: Approx. 2000 times (approx. 2600 times)
CCD camera	Imaging method: EIA Imaging device: 1/3-inch interline CCD External dimensions: 31 (W) × 72.5 (D) × 29 (H) mm Mass: 85g
TFT monitor	Screen size: 210.4 mm diagonal (8.4-inch) Number of pixels: 640 (H) × 480 (V) Rotation range: 350° Tilting range: -5-40° Power supply: AC100-230V50/60Hz Power consumption: 12VA External dimensions: 228 (W) × 61.5 (D) × 195 (H) mm [232 (W) × 227 (D) × 426.5 (H) mm (when installed on the stand)] Mass: 1.8 g (4.2 kg including the stand)

Mitutoyo

Mitutoyo Asia Pacific Pte. Ltd.

Company Reg No. 197800892N

24 Kallang Avenue, Mitutoyo Building, Singapore 339415

Tel: (65) 6294 2211 Fax: (65) 6299 6666

E-mail: mapsg@mitutoyo.com.sg

Export permission by the Japanese government may be required for exporting our products according to the Foreign Exchange and Foreign Trade Law. Please consult our sales office near you before you export our products or you offer technical information to a nonresident.



www.mitutoyo.com.sg | www.mitutoyo.com.my
www.mitutoyo.co.th | www.mitutoyo.co.id
www.mitutoyo.com.vn | www.mitutoyo.com.ph

Mitutoyo (Malaysia) Sdn. Bhd.

Mah Sing Integrated Industrial Park,
4, Jalan Utarid U5/14, Section U5,
40150 Shah Alam, Selangor, Malaysia
Tel: (60) 3-7845 9318
Fax: (60) 3-7845 9346

E-mail: mmsb@mitutoyo.com.my

Penang Branch

Tel: (60) 4-641 1998 Fax: (60) 4-641 2998

Johor Branch

Tel: (60) 7-352 1626 Fax: (60) 7-352 1628

Mitutoyo (Thailand) Co., Ltd.

76/3-5, Chaengwattana Road, Kwaeng
Anusaowaree, Khet Bangkaen,
Bangkok 10220, Thailand
Tel: (66) 2080 3500
Fax: (66) 2521 6136

E-mail: office@mitutoyo.co.th

Chonburi Branch

Tel: (66) 2080 3563 Fax: (66) 3834 5788

ACC Branch

Tel: (66) 2080 3565

PT. Mitutoyo Indonesia

Jalan Sriwijaya No.26
Desa cibatu
Kec. Cikarang Selatan
Kab. Bekasi 17530, Indonesia
Tel: (62) 21-2962 8600
Fax: (62) 21-2962 8604

E-mail: ptmi@mitutoyo.co.id

Mitutoyo Vietnam Co., Ltd.

1st & 2nd Floor, MHD1 Building,
No. 60 Hoang Quoc Viet Road,
Nghia Do Ward, Cau Giay District,
Hanoi, Vietnam
Tel: (84) 24-3768 8963
Fax: (84) 24-3768 8960

E-mail: mvc@mitutoyo.com.vn

Ho Chi Minh City Branch

Tel: (84) 28-3840 3489

Fax: (84) 28-3840 3498

E-mail: mvc@mitutoyo.com.vn

Mitutoyo Philippines, Inc.

Unit 1B & 2B LTT,
Administration Building 1,
Annex 1, North Main Avenue,
Laguna Technopark, Biñan,
Laguna 4024, Philippines
Tel: (63) 49-544 0272
Fax: (63) 49-544 0272

E-mail: mpi@mitutoyo.com.ph

MAP•1319(3)